

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061419\
 Data File : VV011522.D
 Acq On : 15 Jun 2019 06:08
 Operator : SY/MD
 Sample : K3314-18
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COM50

Quant Time: Jun 15 06:38:49 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 15 04:37:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	187814	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	173842	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	69590	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	59474	4.20	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.00%
7) Chloroethane-d5	1.58	69	47037	5.23	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.60%
11) 1,1-Dichloroethene-d2	2.12	63	91285	3.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.60%
20) 2-Butanone-d5	3.97	46	178564	44.75	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.50%
24) Chloroform-d	4.40	84	118359	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.80%
26) 1,2-Dichloroethane-d4	5.08	65	71482	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.80%
32) Benzene-d6	5.09	84	237724	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.60%
36) 1,2-Dichloropropane-d6	6.12	67	73906	4.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.80%
41) Toluene-d8	7.36	98	203944	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.20%
43) trans-1,3-Dichloropropene-	7.66	79	21506	3.92	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.40%
46) 2-Hexanone-d5	8.14	63	140363	44.40	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.80%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	51191	4.15	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	65858	4.74	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.80%


Target Compounds					Ovalue
13) Acetone	2.23	43	7309	2.718 ug/L	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061419\
Data File : VV011522.D
Acq On : 15 Jun 2019 06:08
Operator : SY/MD
Sample : K3314-18
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM50

Quant Time: Jun 15 06:38:49 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 15 04:37:55 2019
Response via : Initial Calibration

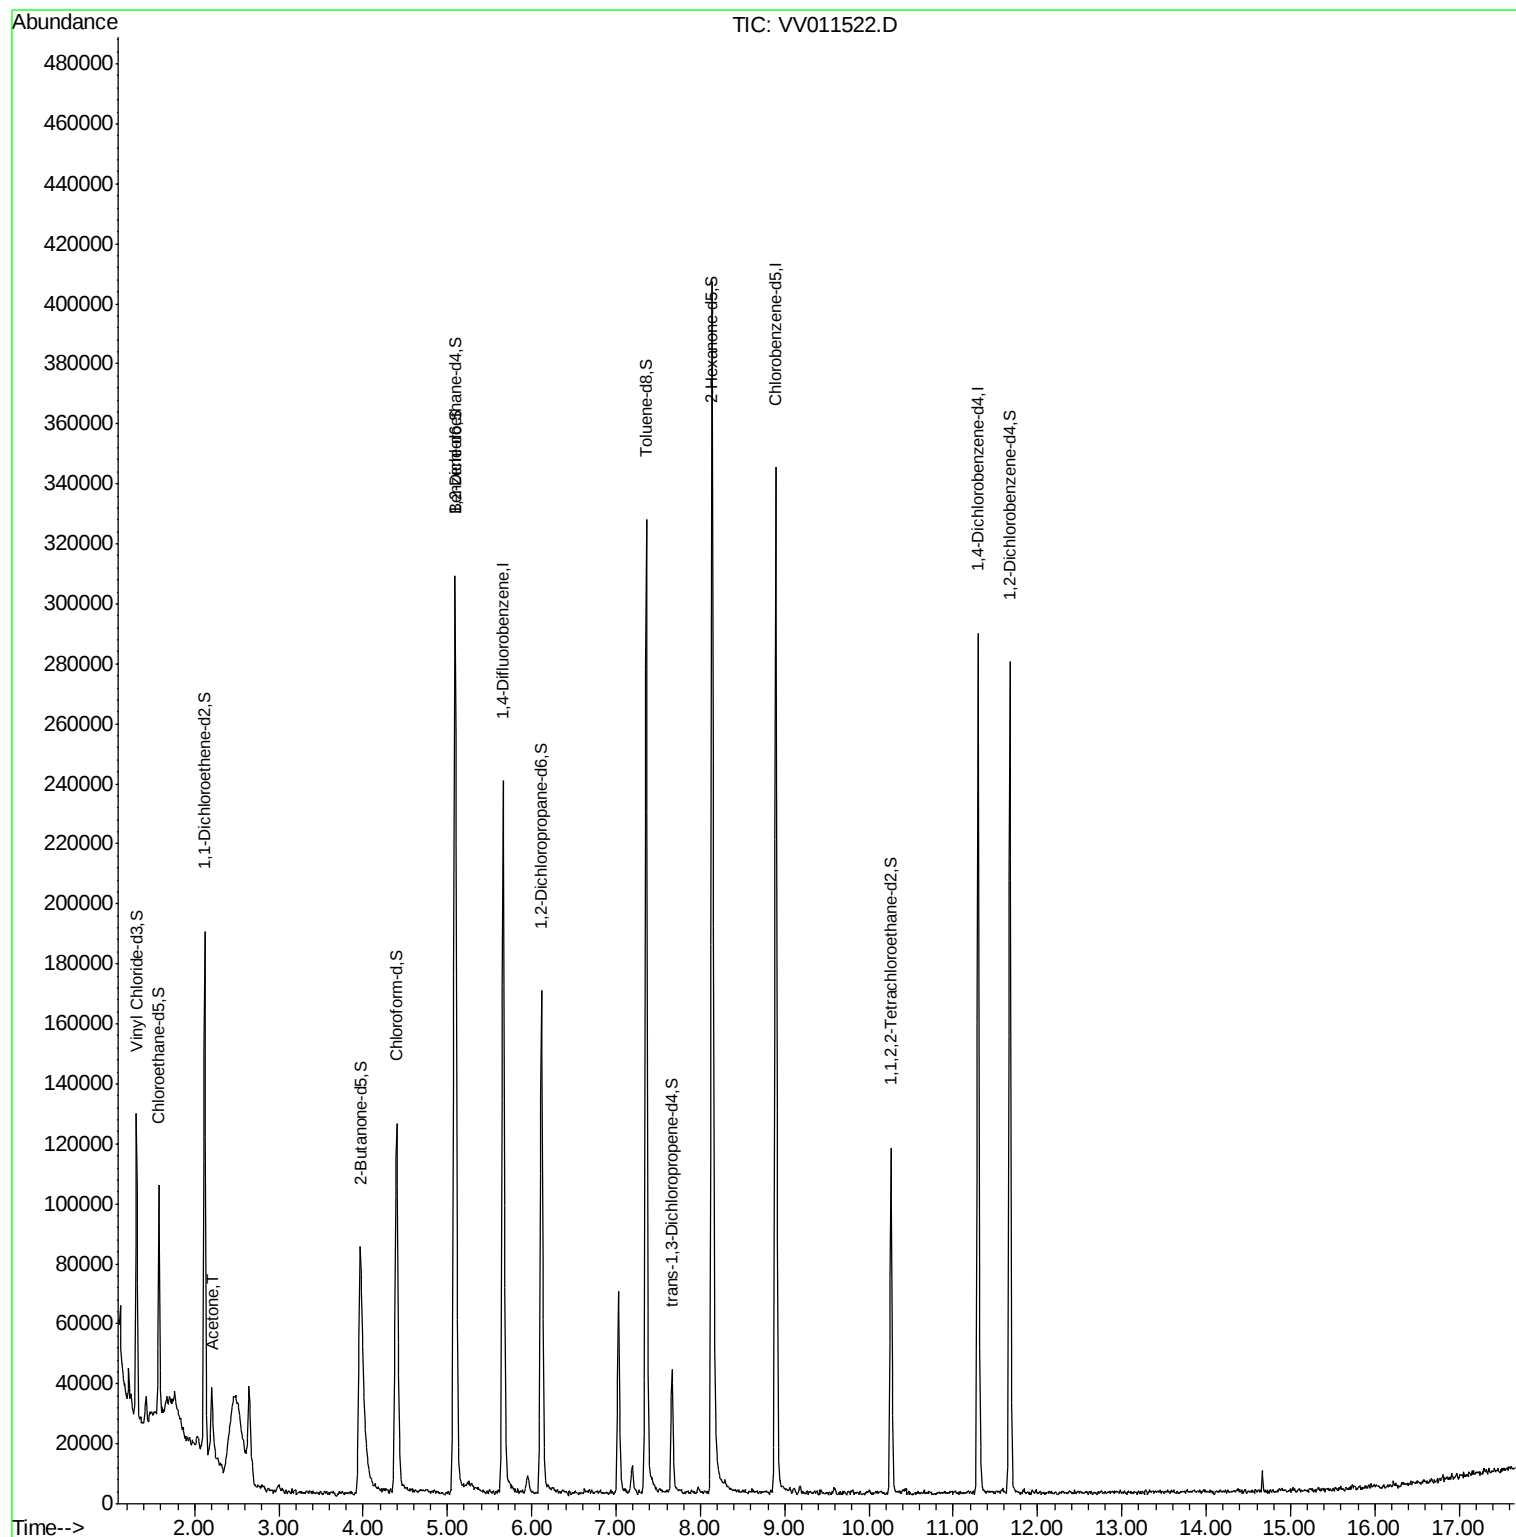

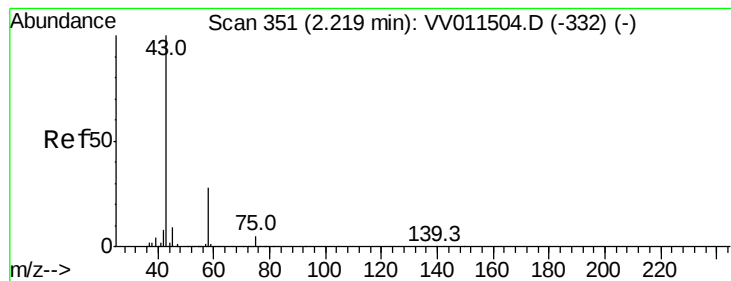

#13

Acetone

Concen: 2.718 ug/L

RT: 2.23 min Scan# 353

Delta R.T. 0.01 min

Lab File: VV011522.D

Acq: 15 Jun 2019 06:08

Instrument :

MSVOA_V

ClientSampleId :

COM50

Tot Ion: 43 Resp: 7309

Ion Ratio Lower Upper

43 100

58 16.9 0.0 57.8

