

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061419\
 Data File : VV011537.D
 Acq On : 15 Jun 2019 14:09
 Operator : SY/MD
 Sample : K3386-02
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COM74

Quant Time: Jun 17 07:04:38 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 17 04:30:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	188481	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	171102	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	66627	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	61673	4.34	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.80%
7) Chloroethane-d5	1.58	69	46521	5.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.20%
11) 1,1-Dichloroethene-d2	2.12	63	94490	3.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.80%
20) 2-Butanone-d5	3.95	46	191069	47.72	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.44%
24) Chloroform-d	4.40	84	124277	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.80%
26) 1,2-Dichloroethane-d4	5.08	65	74648	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.80%
32) Benzene-d6	5.09	84	247583	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.00%
36) 1,2-Dichloropropane-d6	6.12	67	77513	4.78	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.60%
41) Toluene-d8	7.36	98	211274	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.80%
43) trans-1,3-Dichloropropene-	7.66	79	21441	3.98	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.60%
46) 2-Hexanone-d5	8.14	63	144362	46.39	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.78%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	53261	4.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	68309	5.14	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.80%


Target Compounds					Ovalue
13) Acetone	2.21	43	7540	2.794 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061419\
Data File : VV011537.D
Acq On : 15 Jun 2019 14:09
Operator : SY/MD
Sample : K3386-02
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM74

Quant Time: Jun 17 07:04:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 17 04:30:15 2019
Response via : Initial Calibration

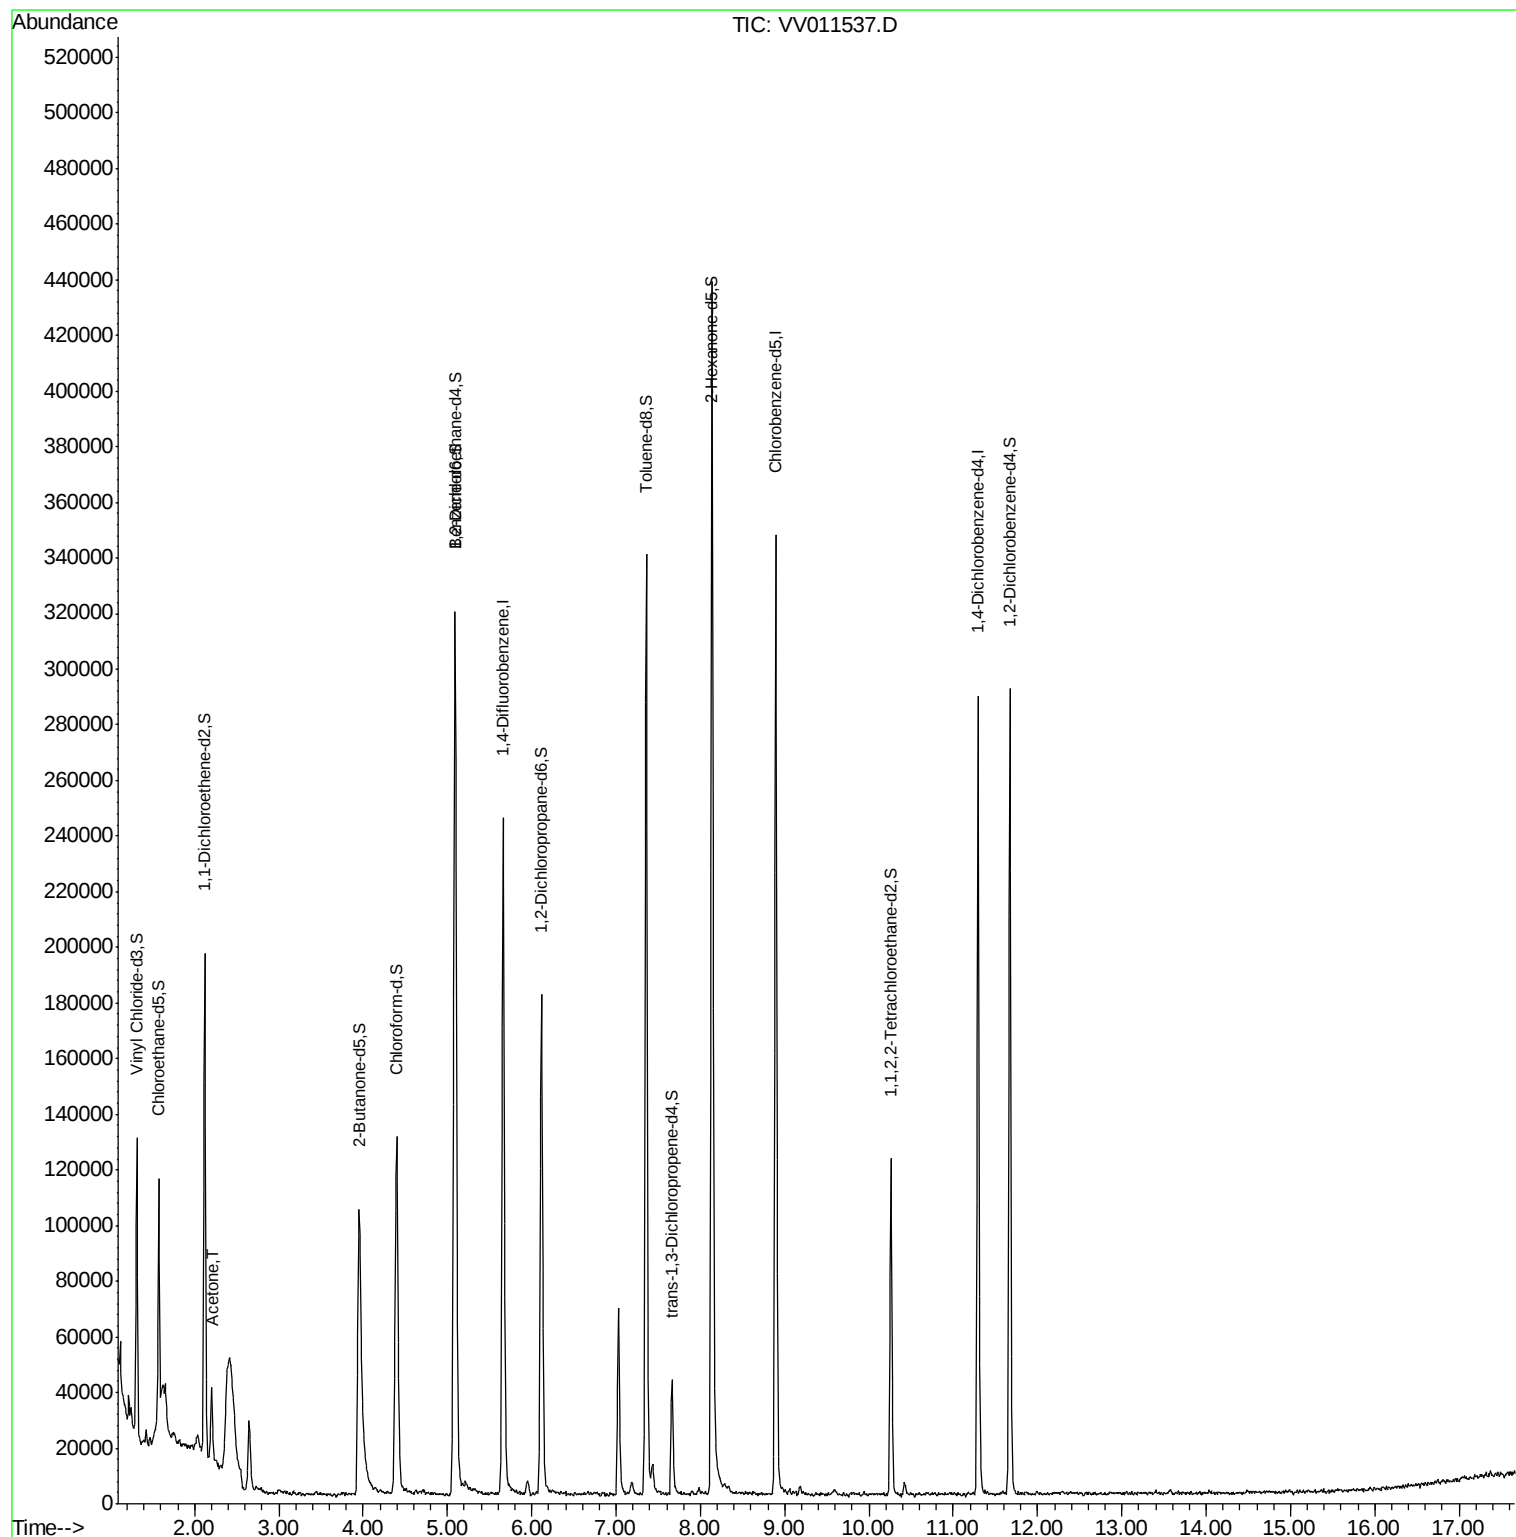

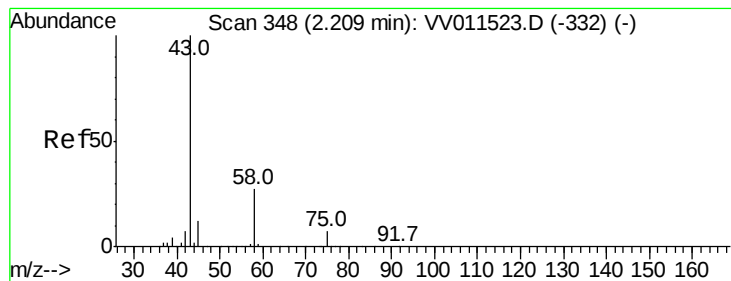

#13
 Acetone
 Concen: 2.794 ug/L
 RT: 2.21 min Scan# 349
 Delta R.T. 0.00 min
 Lab File: VV011537.D
 Acq: 15 Jun 2019 14:09

Instrument :
 MSVOA_V
 ClientSampleId :
 COM74

Tot Ion: 43 Resp: 7540
 Ion Ratio Lower Upper
 43 100
 58 34.1 0.0 57.8

