

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061422\
 Data File : VW026226.D
 Acq On : 14 Jun 2022 10:57
 Operator : SY/MD
 Sample : N3312-18
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jun 15 05:47:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 15 05:46:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	166688	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	165293	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	65556	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.314	65	93018	4.267	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.400%
7) Chloroethane-d5	1.574	69	76945	4.482	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.600%
11) 1,1-Dichloroethene-d2	2.114	63	121302	3.461	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.200%
20) 2-Butanone-d5	3.902	46	68485	42.112	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.220%
24) Chloroform-d	4.352	84	137213	4.439	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.800%
26) 1,2-Dichloroethane-d4	5.034	65	58238	4.673	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.400%
32) Benzene-d6	5.053	84	267096	4.145	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.800%
36) 1,2-Dichloropropane-d6	6.069	67	83140	4.474	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.400%
41) Toluene-d8	7.317	98	213281	3.717	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.400%
43) trans-1,3-Dichloroprop...	7.625	79	19745	3.520	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.400%
46) 2-Hexanone-d5	8.088	63	69356	39.715	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.420%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	44791	4.046	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	68832	4.684	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.600%
Target Compounds						Qvalue
16) Methylene chloride	2.513	84	17486	1.331	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026226.D
Acq On : 14 Jun 2022 10:57
Operator : SY/MD
Sample : N3312-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Jun 15 05:47:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 15 05:46:56 2022
Response via : Initial Calibration

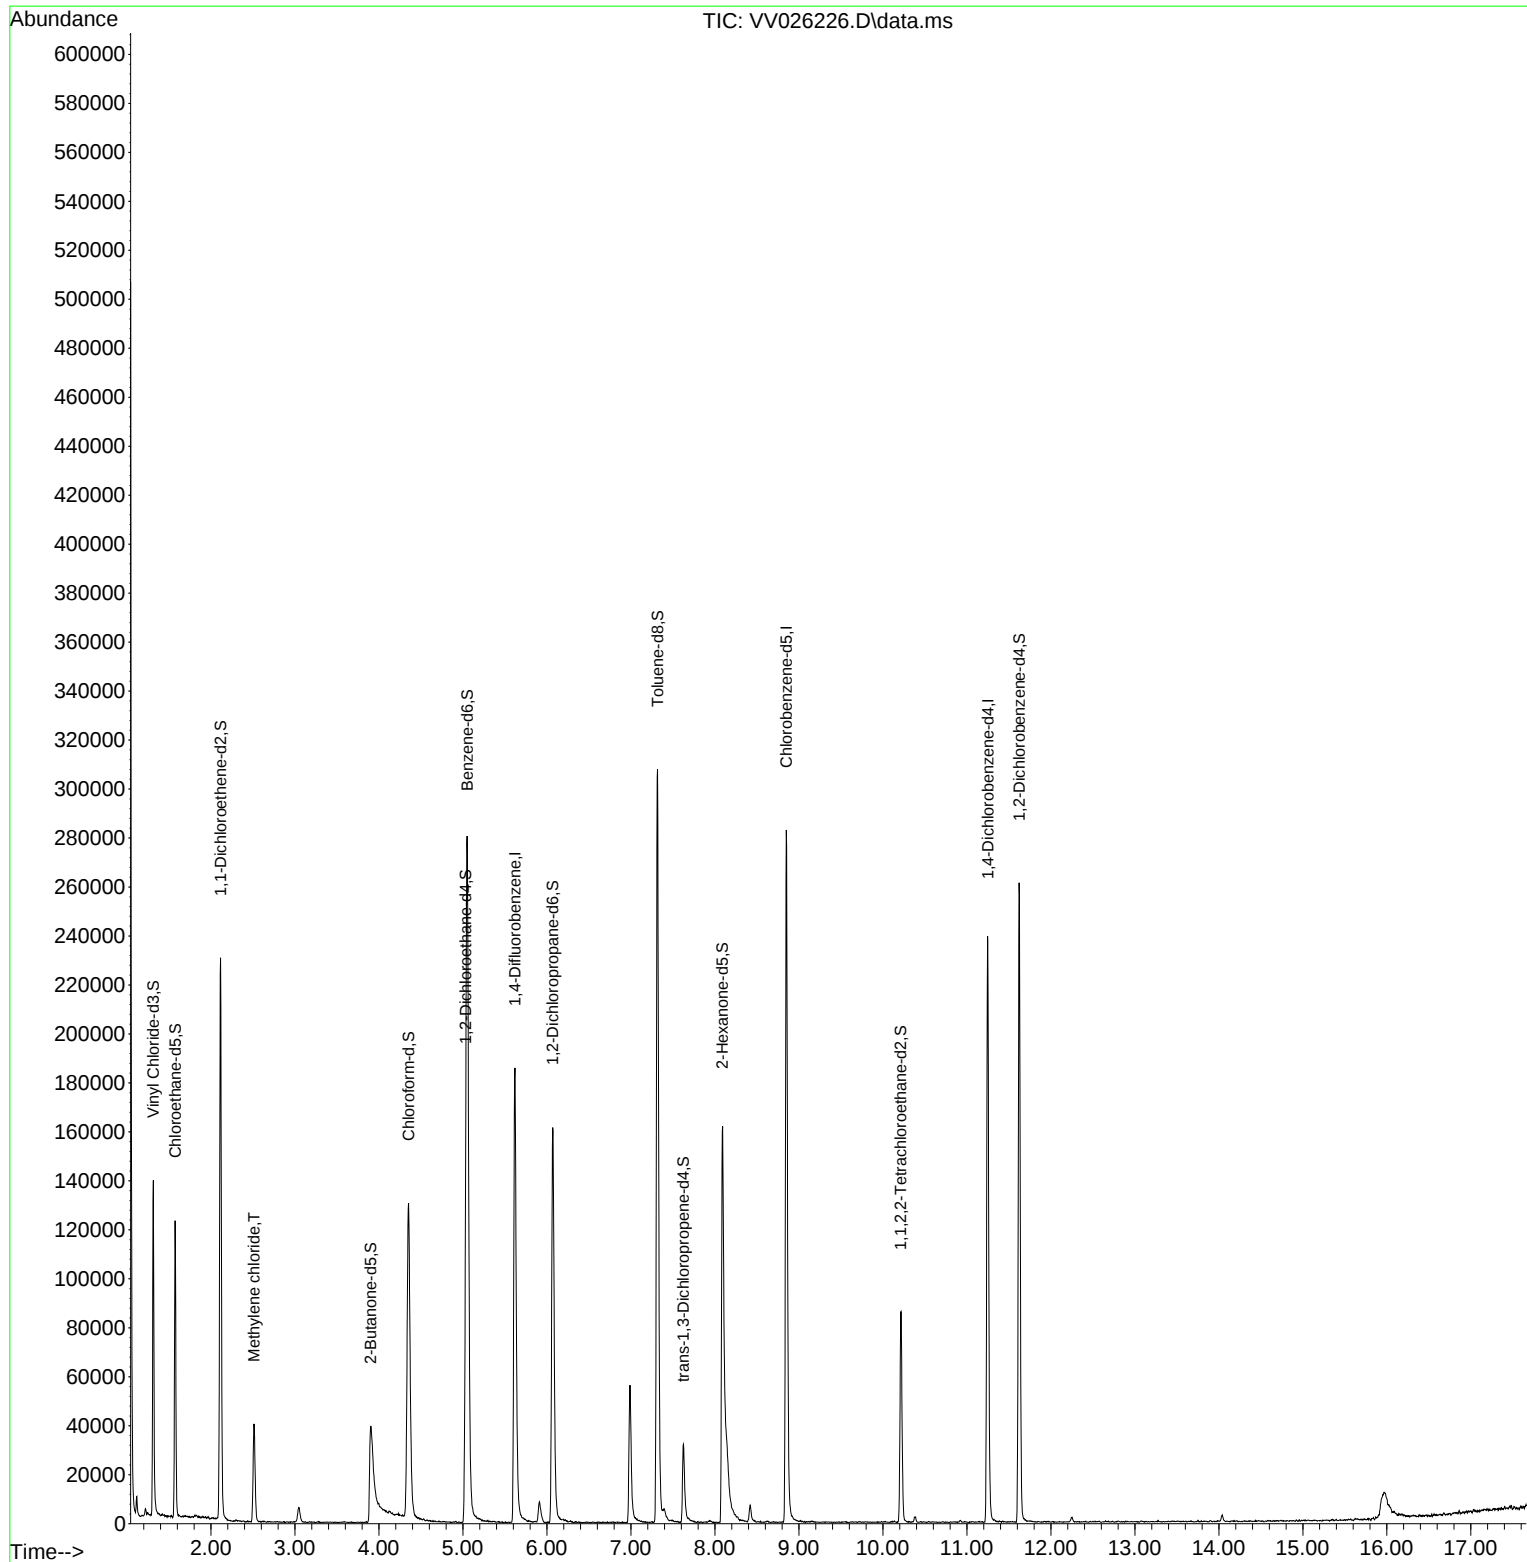

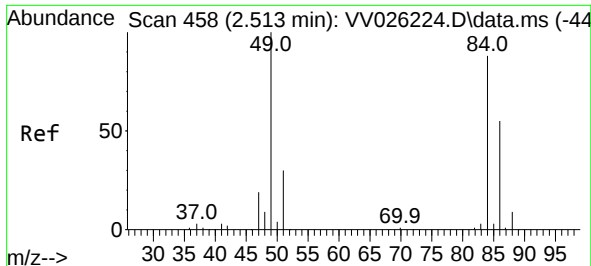

#16
Methylene chloride
Concen: 1.331 ug/L
RT: 2.513 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV026226.D
Acq: 14 Jun 2022 10:57

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

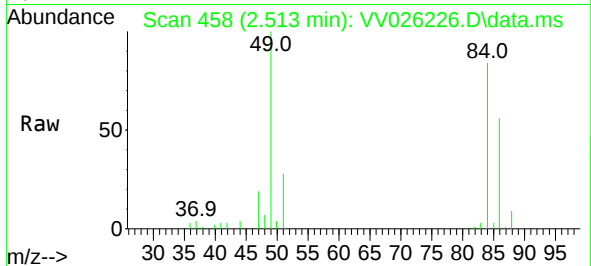

Tgt Ion: 84 Resp: 17486

Ion	Ratio	Lower	Upper
84	100		
86	66.7	45.1	83.7
49	118.5	82.3	152.9

