

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061422\
 Data File : VW026232.D
 Acq On : 14 Jun 2022 13:20
 Operator : SY/MD
 Sample : N3312-18
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jun 15 05:49:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 15 05:46:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	167933	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	165685	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	66418	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.314	65	93354	4.251	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.000%
7) Chloroethane-d5	1.574	69	81063	4.686	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.800%
11) 1,1-Dichloroethene-d2	2.114	63	126361	3.578	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.600%
20) 2-Butanone-d5	3.912	46	101082	61.696	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	123.400%
24) Chloroform-d	4.355	84	153920	4.942	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.800%
26) 1,2-Dichloroethane-d4	5.037	65	68252	5.436	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.800%
32) Benzene-d6	5.056	84	300183	4.647	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.000%
36) 1,2-Dichloropropane-d6	6.072	67	92548	4.969	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.400%
41) Toluene-d8	7.317	98	235740	4.099	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.000%
43) trans-1,3-Dichloroprop...	7.625	79	26602	4.732	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.600%
46) 2-Hexanone-d5	8.091	63	96176	54.942	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.880%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	54556	4.916	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.400%
66) 1,2-Dichlorobenzene-d4	11.625	152	78973	5.304	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.000%
Target Compounds						
16) Methylene chloride	2.516	84	6374	0.482	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026232.D
Acq On : 14 Jun 2022 13:20
Operator : SY/MD
Sample : N3312-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Jun 15 05:49:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 15 05:46:56 2022
Response via : Initial Calibration

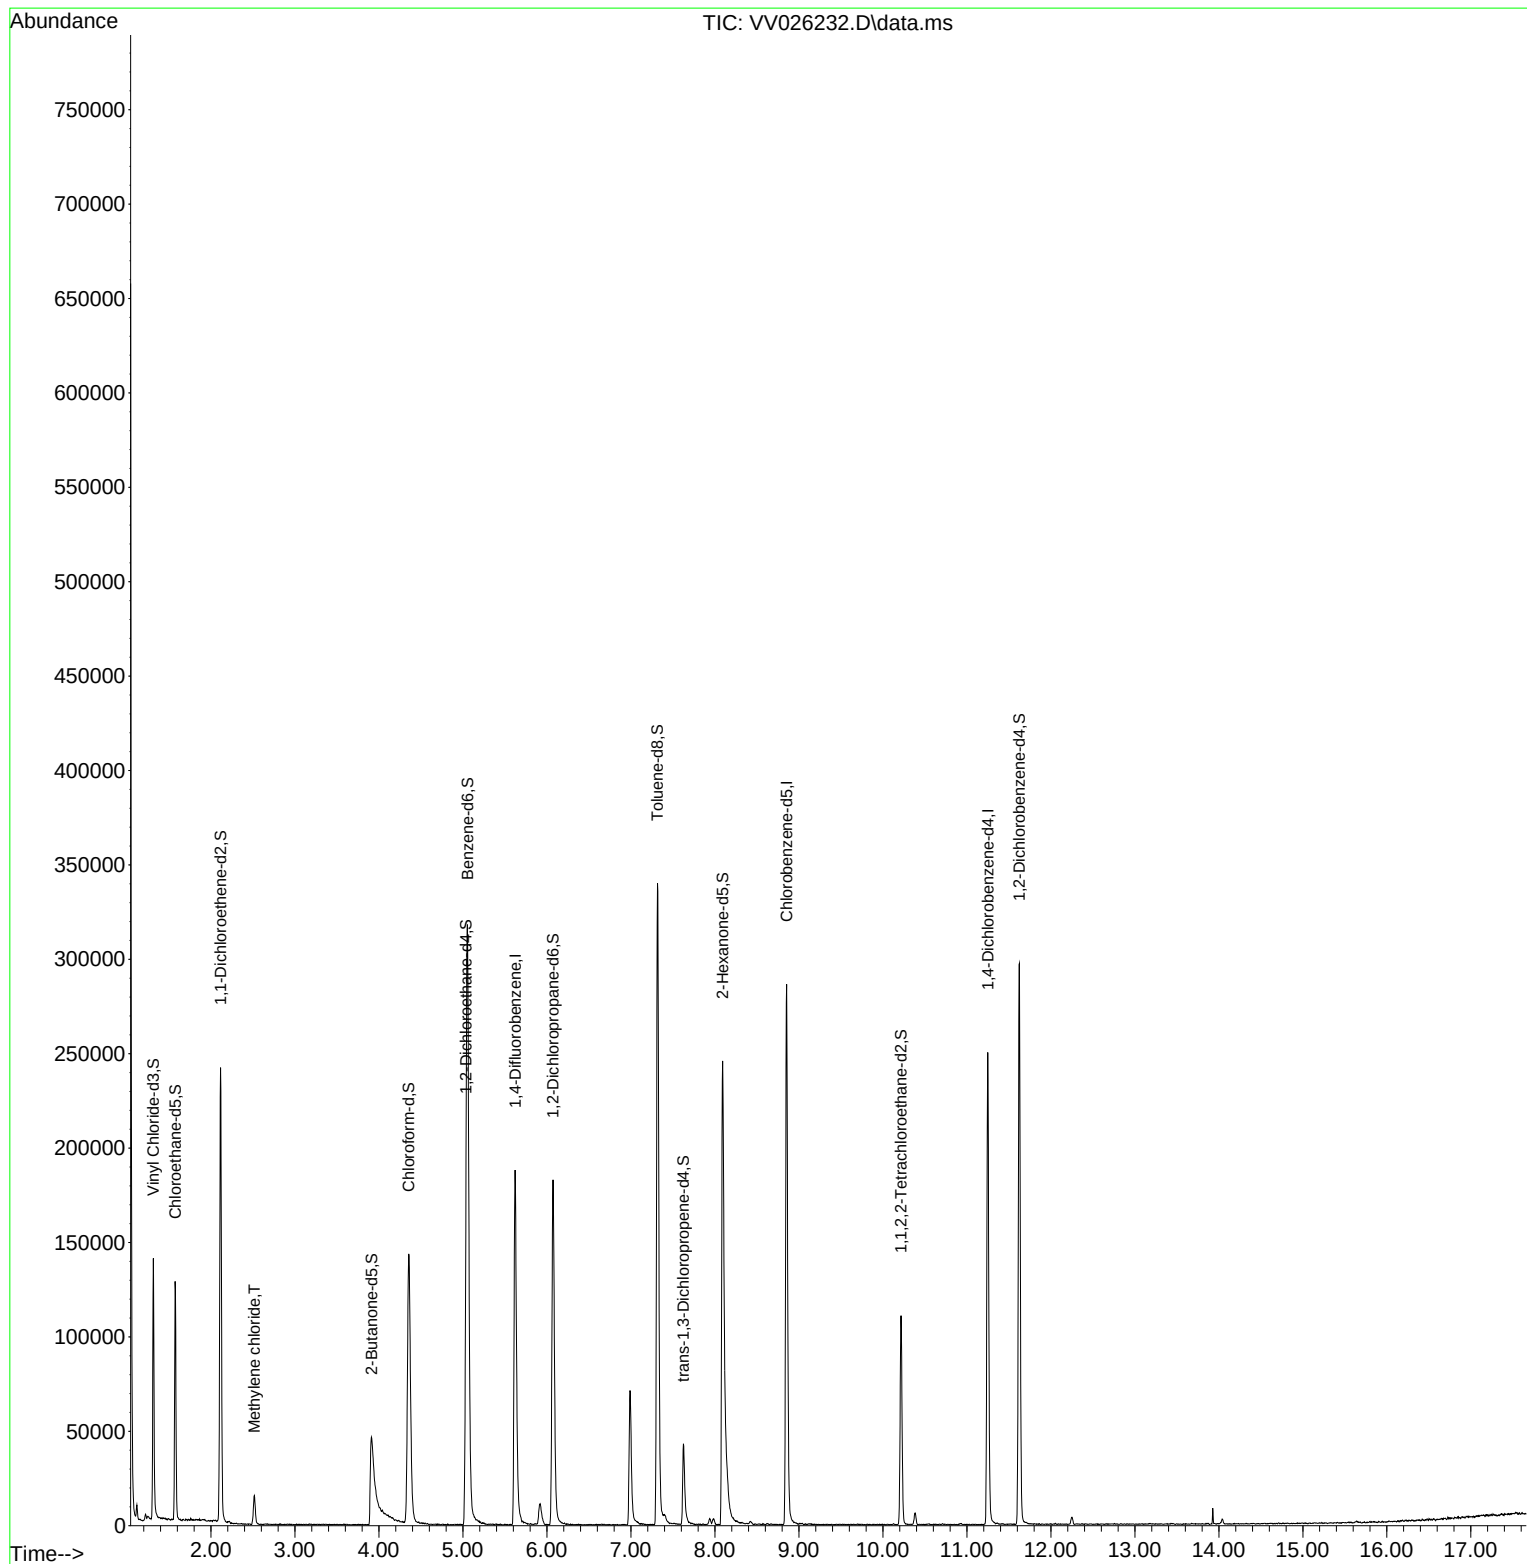

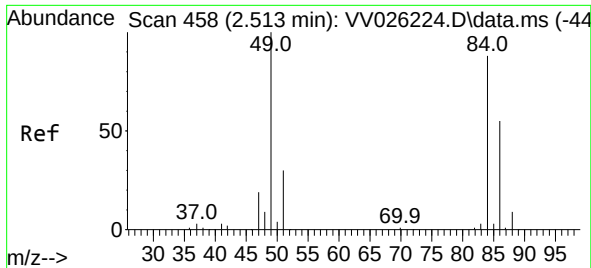

#16
Methylene chloride
Concen: 0.482 ug/L
RT: 2.516 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV026232.D
Acq: 14 Jun 2022 13:20

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

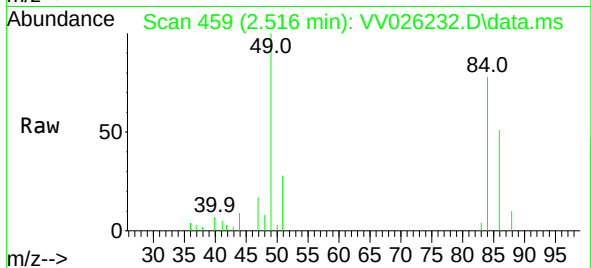

Tgt Ion: 84 Resp: 6374

Ion	Ratio	Lower	Upper
84	100		
86	65.8	45.1	83.7
49	127.9	82.3	152.9

