

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061422\
 Data File : VW026246.D
 Acq On : 14 Jun 2022 19:41
 Operator : SY/MD
 Sample : N3272-21
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jun 15 05:53:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 15 05:46:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	159924	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	157578	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	64529	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.314	65	92898	4.442	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.800%
7) Chloroethane-d5	1.574	69	80834	4.907	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.200%
11) 1,1-Dichloroethene-d2	2.114	63	124141	3.692	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.800%
20) 2-Butanone-d5	3.915	46	130035	83.342	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	166.680%#
24) Chloroform-d	4.355	84	152352	5.137	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.800%
26) 1,2-Dichloroethane-d4	5.040	65	67965	5.684	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.600%
32) Benzene-d6	5.053	84	301999	4.916	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.400%
36) 1,2-Dichloropropane-d6	6.072	67	94368	5.327	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.600%
41) Toluene-d8	7.316	98	238057	4.352	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.000%
43) trans-1,3-Dichloroprop...	7.625	79	26082	4.878	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.600%
46) 2-Hexanone-d5	8.091	63	92905	55.804	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.600%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	55344	5.244	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.800%
66) 1,2-Dichlorobenzene-d4	11.625	152	77470	5.356	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.200%
Target Compounds						
					Qvalue	
16) Methylene chloride	2.513	84	5960	0.473	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026246.D
Acq On : 14 Jun 2022 19:41
Operator : SY/MD
Sample : N3272-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Jun 15 05:53:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 15 05:46:56 2022
Response via : Initial Calibration

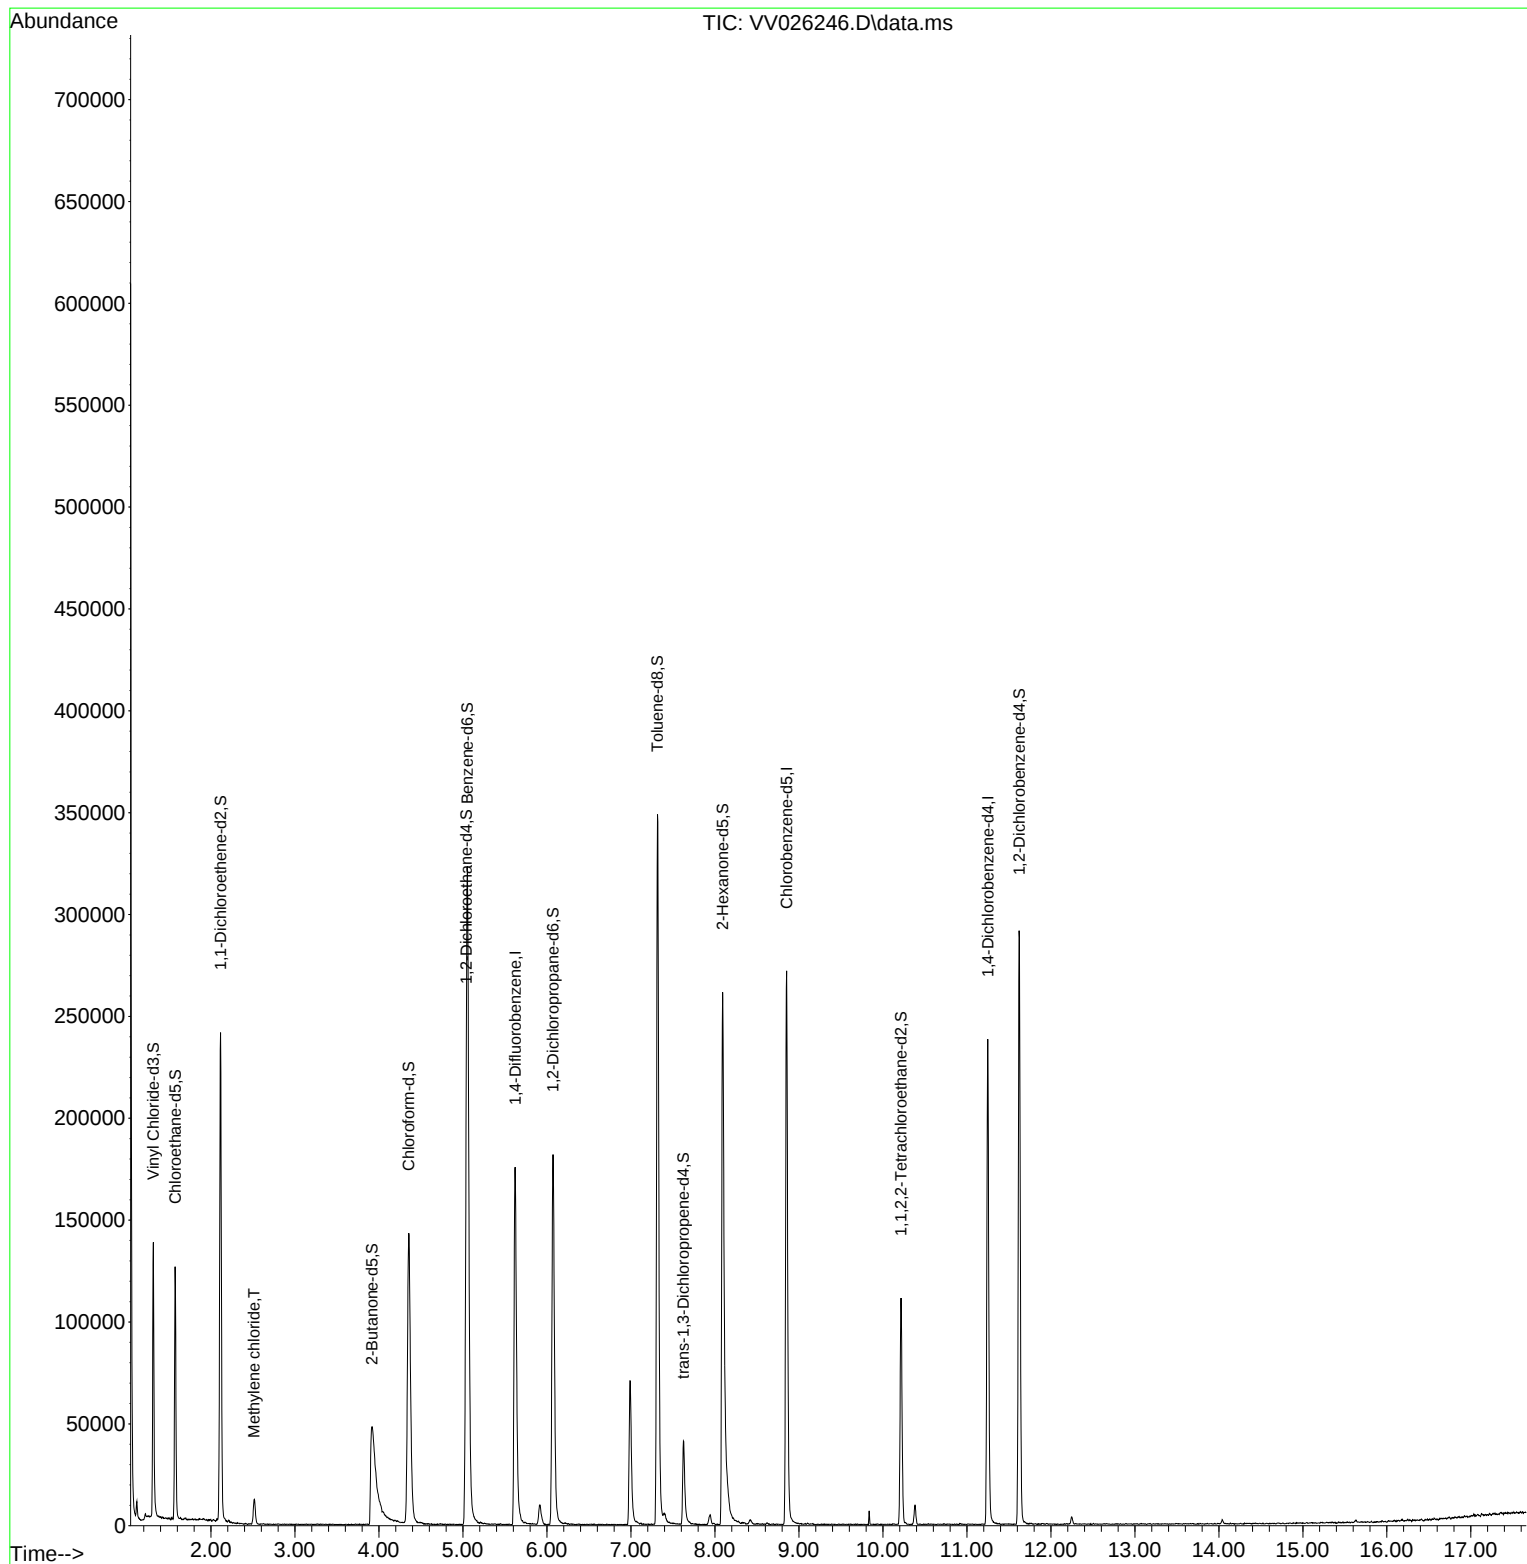

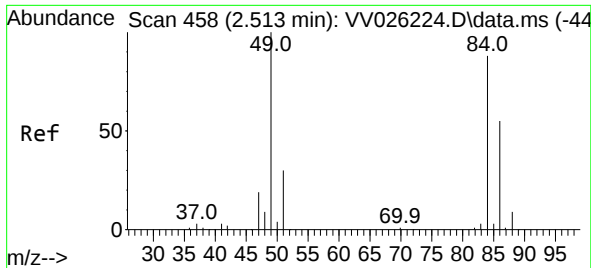

#16
Methylene chloride
Concen: 0.473 ug/L
RT: 2.513 min Scan# 4
Delta R.T. -0.000 min
Lab File: VV026246.D
Acq: 14 Jun 2022 19:41

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

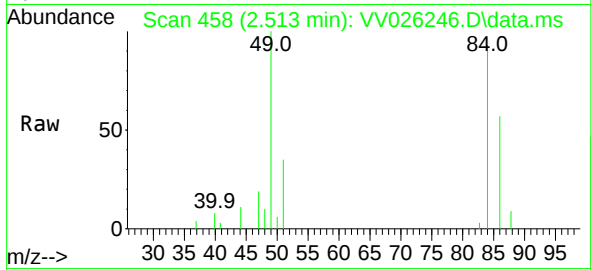

Tgt Ion: 84 Resp: 5960
Ion Ratio Lower Upper
84 100
86 61.2 45.1 83.7
49 107.4 82.3 152.9

