

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061422\
 Data File : VW026248.D
 Acq On : 14 Jun 2022 20:31
 Operator : SY/MD
 Sample : VW0614WBL02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK372

Quant Time: Jun 15 09:39:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 15 07:11:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	178165	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	168545	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	71957	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.314	65	95195	4.086	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.800%
7) Chloroethane-d5	1.574	69	83151	4.531	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.600%
11) 1,1-Dichloroethene-d2	2.111	63	129004	3.443	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.800%
20) 2-Butanone-d5	3.915	46	135804	78.128	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	156.260%#
24) Chloroform-d	4.355	84	159597	4.830	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.600%
26) 1,2-Dichloroethane-d4	5.037	65	72657	5.454	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.000%
32) Benzene-d6	5.053	84	319295	4.859	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.200%
36) 1,2-Dichloropropane-d6	6.069	67	97058	5.122	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.400%
41) Toluene-d8	7.317	98	253496	4.333	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.600%
43) trans-1,3-Dichloroprop...	7.625	79	28215	4.934	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.600%
46) 2-Hexanone-d5	8.092	63	99674	55.974	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.940%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	57760	5.116	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	85504	5.301	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.000%
Target Compounds						Qvalue
16) Methylene chloride	2.516	84	9462	0.674	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026248.D
Acq On : 14 Jun 2022 20:31
Operator : SY/MD
Sample : VV0614WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK372


Quant Time: Jun 15 09:39:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 15 07:11:20 2022
Response via : Initial Calibration

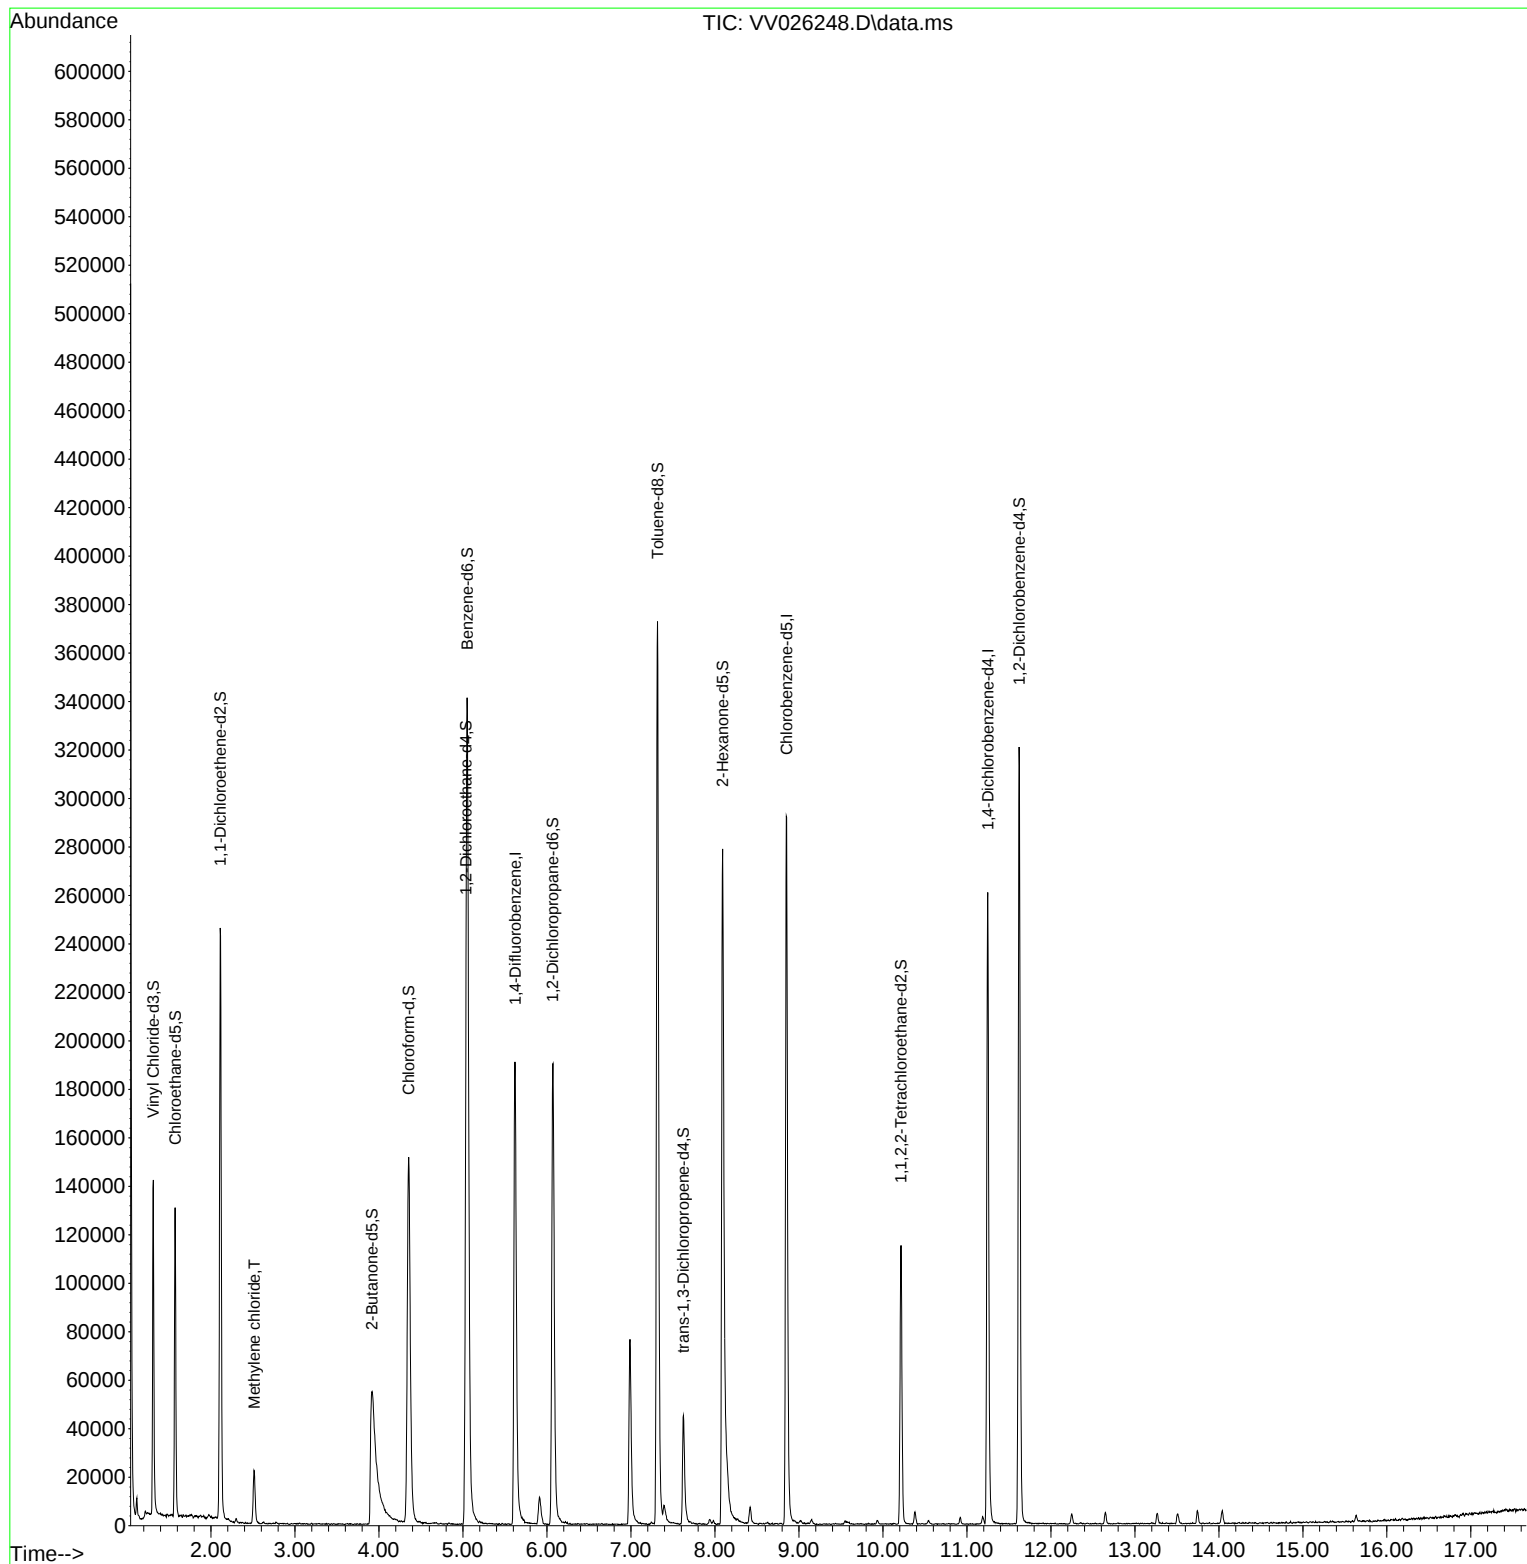

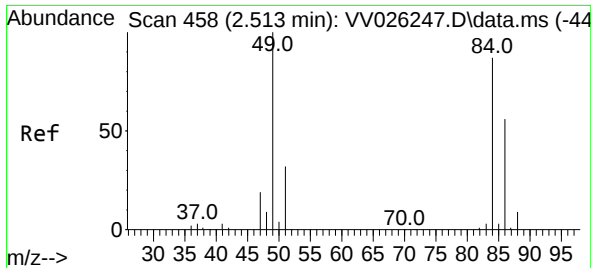

#16
Methylene chloride
Concen: 0.674 ug/L
RT: 2.516 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV026248.D
Acq: 14 Jun 2022 20:31

Instrument :
MSVOA_V
ClientSampleId :
VBLK372

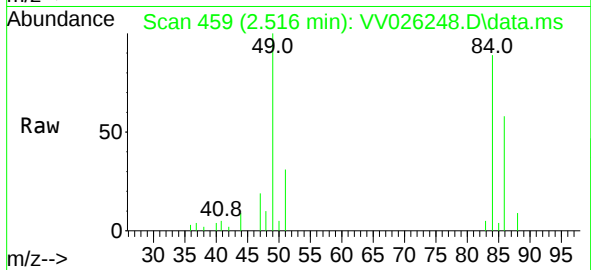

Tgt Ion: 84 Resp: 9462

Ion	Ratio	Lower	Upper
84	100		
86	65.0	45.1	83.7
49	111.9	82.3	152.9

