

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061422\
 Data File : VW026251.D
 Acq On : 14 Jun 2022 22:13
 Operator : SY/MD
 Sample : N3275-03 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD5

Quant Time: Jun 15 09:40:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 15 07:11:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	173862	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	169393	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	70232	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.314	65	88707	3.902	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.000%
7) Chloroethane-d5	1.574	69	76325	4.262	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.200%
11) 1,1-Dichloroethene-d2	2.111	63	120697	3.301	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.000%
20) 2-Butanone-d5	3.905	46	96742	57.033	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.060%
24) Chloroform-d	4.352	84	153016	4.746	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.000%
26) 1,2-Dichloroethane-d4	5.034	65	67242	5.173	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.400%
32) Benzene-d6	5.053	84	295549	4.475	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.600%
36) 1,2-Dichloropropane-d6	6.069	67	92422	4.853	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.000%
41) Toluene-d8	7.317	98	232877	3.960	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.200%
43) trans-1,3-Dichloroprop...	7.625	79	25331	4.407	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.200%
46) 2-Hexanone-d5	8.088	63	91042	50.871	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.740%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	53233	4.692	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	78569	4.991	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.800%
Target Compounds						
					Qvalue	
16) Methylene chloride	2.513	84	2684	0.196	ug/L	96
25) Chloroform	4.381	83	6055	0.237	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026251.D
Acq On : 14 Jun 2022 22:13
Operator : SY/MD
Sample : N3275-03 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD5

Quant Time: Jun 15 09:40:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 15 07:11:20 2022
Response via : Initial Calibration




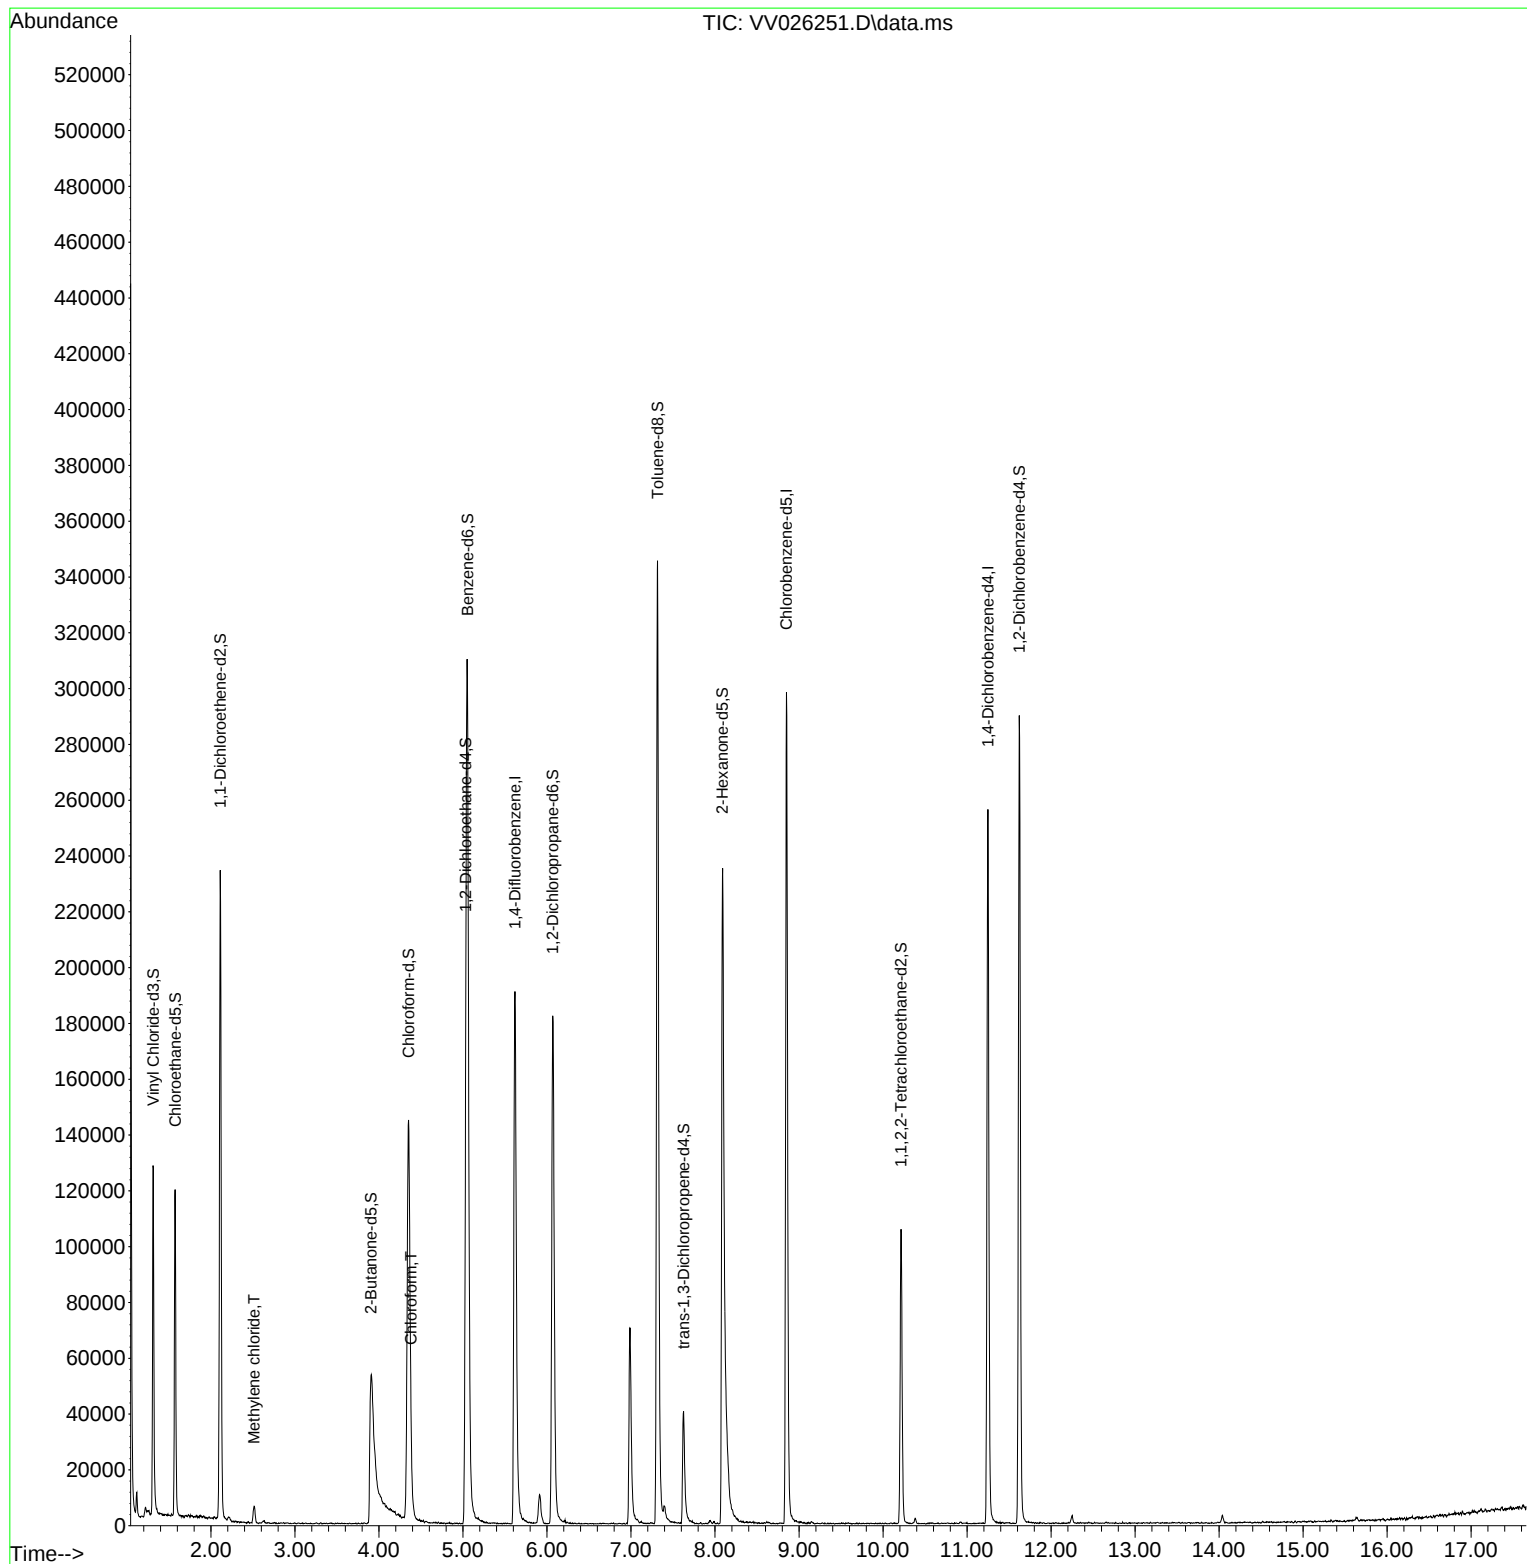


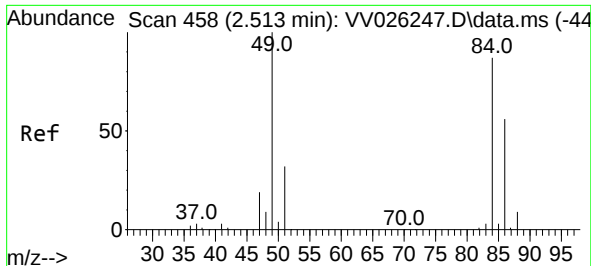

#16
Methylene chloride
Concen: 0.196 ug/L
RT: 2.513 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV026251.D
Acq: 14 Jun 2022 22:13

Instrument :
MSVOA_V
ClientSampleId :
C0BD5

Tgt Ion: 84 Resp: 2684
Ion Ratio Lower Upper
84 100
86 66.9 45.1 83.7
49 112.5 82.3 152.9

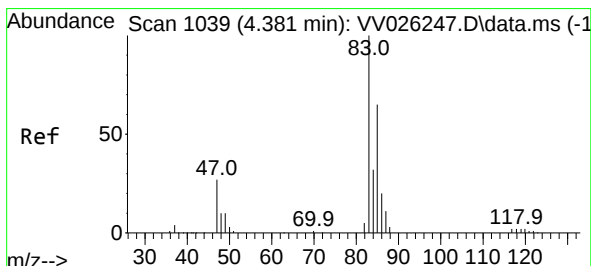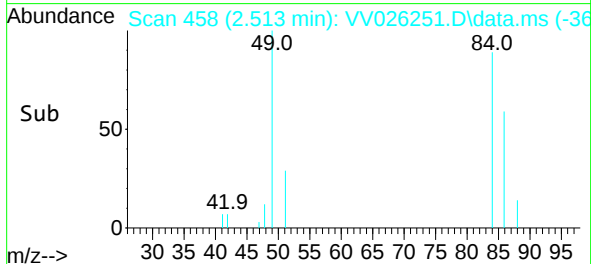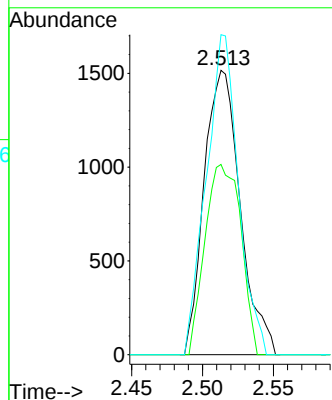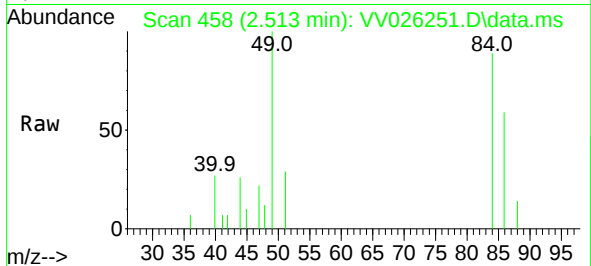

#25
Chloroform
Concen: 0.237 ug/L
RT: 4.381 min Scan# 1039
Delta R.T. 0.000 min
Lab File: VV026251.D
Acq: 14 Jun 2022 22:13

Tgt Ion: 83 Resp: 6055
Ion Ratio Lower Upper
83 100
85 70.2 45.3 84.1

