

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061422\
 Data File : VW026252.D
 Acq On : 14 Jun 2022 22:36
 Operator : SY/MD
 Sample : N3275-04 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD6

Quant Time: Jun 15 09:40:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 15 07:11:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	169451	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	162696	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	66803	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.314	65	85521	3.859	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	77.200%	
7) Chloroethane-d5	1.574	69	74483	4.267	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	85.400%	
11) 1,1-Dichloroethene-d2	2.114	63	115775	3.249	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	65.000%	
20) 2-Butanone-d5	3.912	46	112452	68.020	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	136.040%#	
24) Chloroform-d	4.355	84	147894	4.706	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.200%	
26) 1,2-Dichloroethane-d4	5.037	65	67544	5.331	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	106.600%	
32) Benzene-d6	5.056	84	290179	4.575	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.400%	
36) 1,2-Dichloropropane-d6	6.072	67	90065	4.924	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	98.400%	
41) Toluene-d8	7.317	98	229388	4.062	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	81.200%	
43) trans-1,3-Dichloroprop...	7.625	79	25019	4.532	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.600%	
46) 2-Hexanone-d5	8.092	63	93708	54.516	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	109.040%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	55859	5.126	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	102.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	77551	5.179	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	103.600%	
Target Compounds					Qvalue	
25) Chloroform	4.381	83	6986	0.280	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026252.D
Acq On : 14 Jun 2022 22:36
Operator : SY/MD
Sample : N3275-04 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD6

Quant Time: Jun 15 09:40:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 15 07:11:20 2022
Response via : Initial Calibration

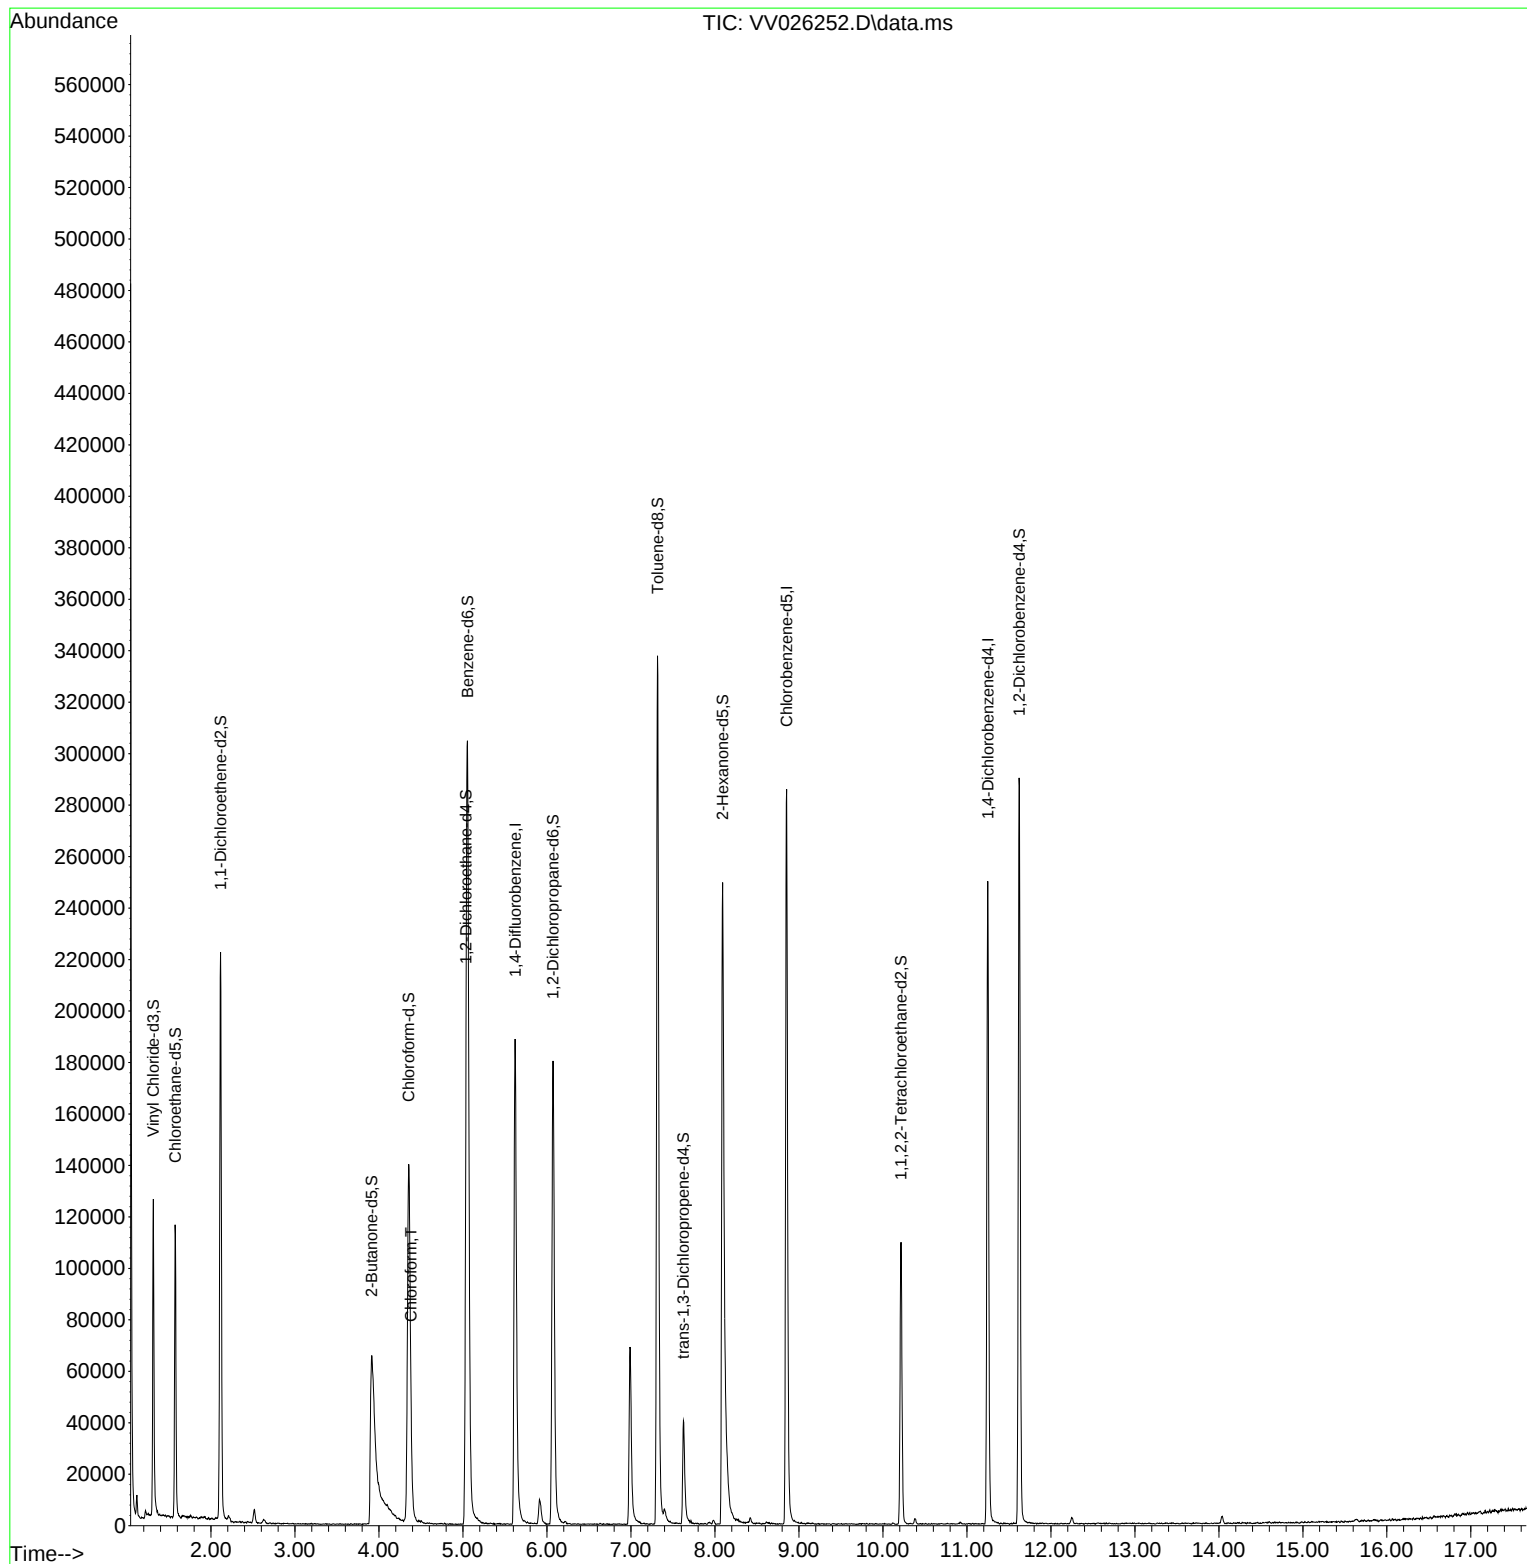

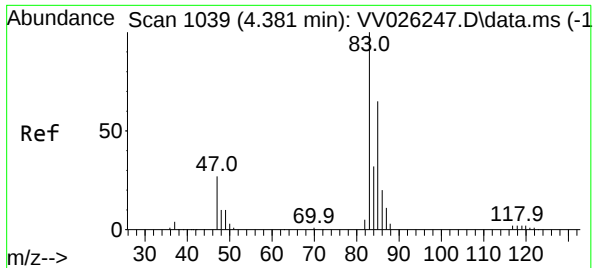

#25
Chloroform
Concen: 0.280 ug/L
RT: 4.381 min Scan# 10
Delta R.T. 0.000 min
Lab File: VV026252.D
Acq: 14 Jun 2022 22:36

Instrument :
MSVOA_V
ClientSampleId :
C0BD6

Tgt Ion: 83 Resp: 6986
Ion Ratio Lower Upper
83 100
85 71.2 45.3 84.1

