

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061422\
 Data File : VW026253.D
 Acq On : 14 Jun 2022 23:00
 Operator : SY/MD
 Sample : N3275-05 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD7

Quant Time: Jun 15 09:40:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 15 07:11:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	163509	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	158737	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	65670	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.314	65	84123	3.934	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.600%
7) Chloroethane-d5	1.574	69	74307	4.412	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.200%
11) 1,1-Dichloroethene-d2	2.114	63	115960	3.373	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.400%
20) 2-Butanone-d5	3.912	46	101282	63.490	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	126.980%
24) Chloroform-d	4.355	84	149679	4.936	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.800%
26) 1,2-Dichloroethane-d4	5.037	65	65618	5.367	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.400%
32) Benzene-d6	5.056	84	286766	4.634	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.600%
36) 1,2-Dichloropropane-d6	6.072	67	90143	5.051	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.000%
41) Toluene-d8	7.317	98	227118	4.122	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.400%
43) trans-1,3-Dichloroprop...	7.625	79	25008	4.643	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.800%
46) 2-Hexanone-d5	8.092	63	90803	54.143	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.280%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	54330	5.110	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	78601	5.340	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.800%
Target Compounds					Qvalue	
25) Chloroform	4.384	83	6477	0.269	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026253.D
Acq On : 14 Jun 2022 23:00
Operator : SY/MD
Sample : N3275-05 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD7

Quant Time: Jun 15 09:40:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 15 07:11:20 2022
Response via : Initial Calibration

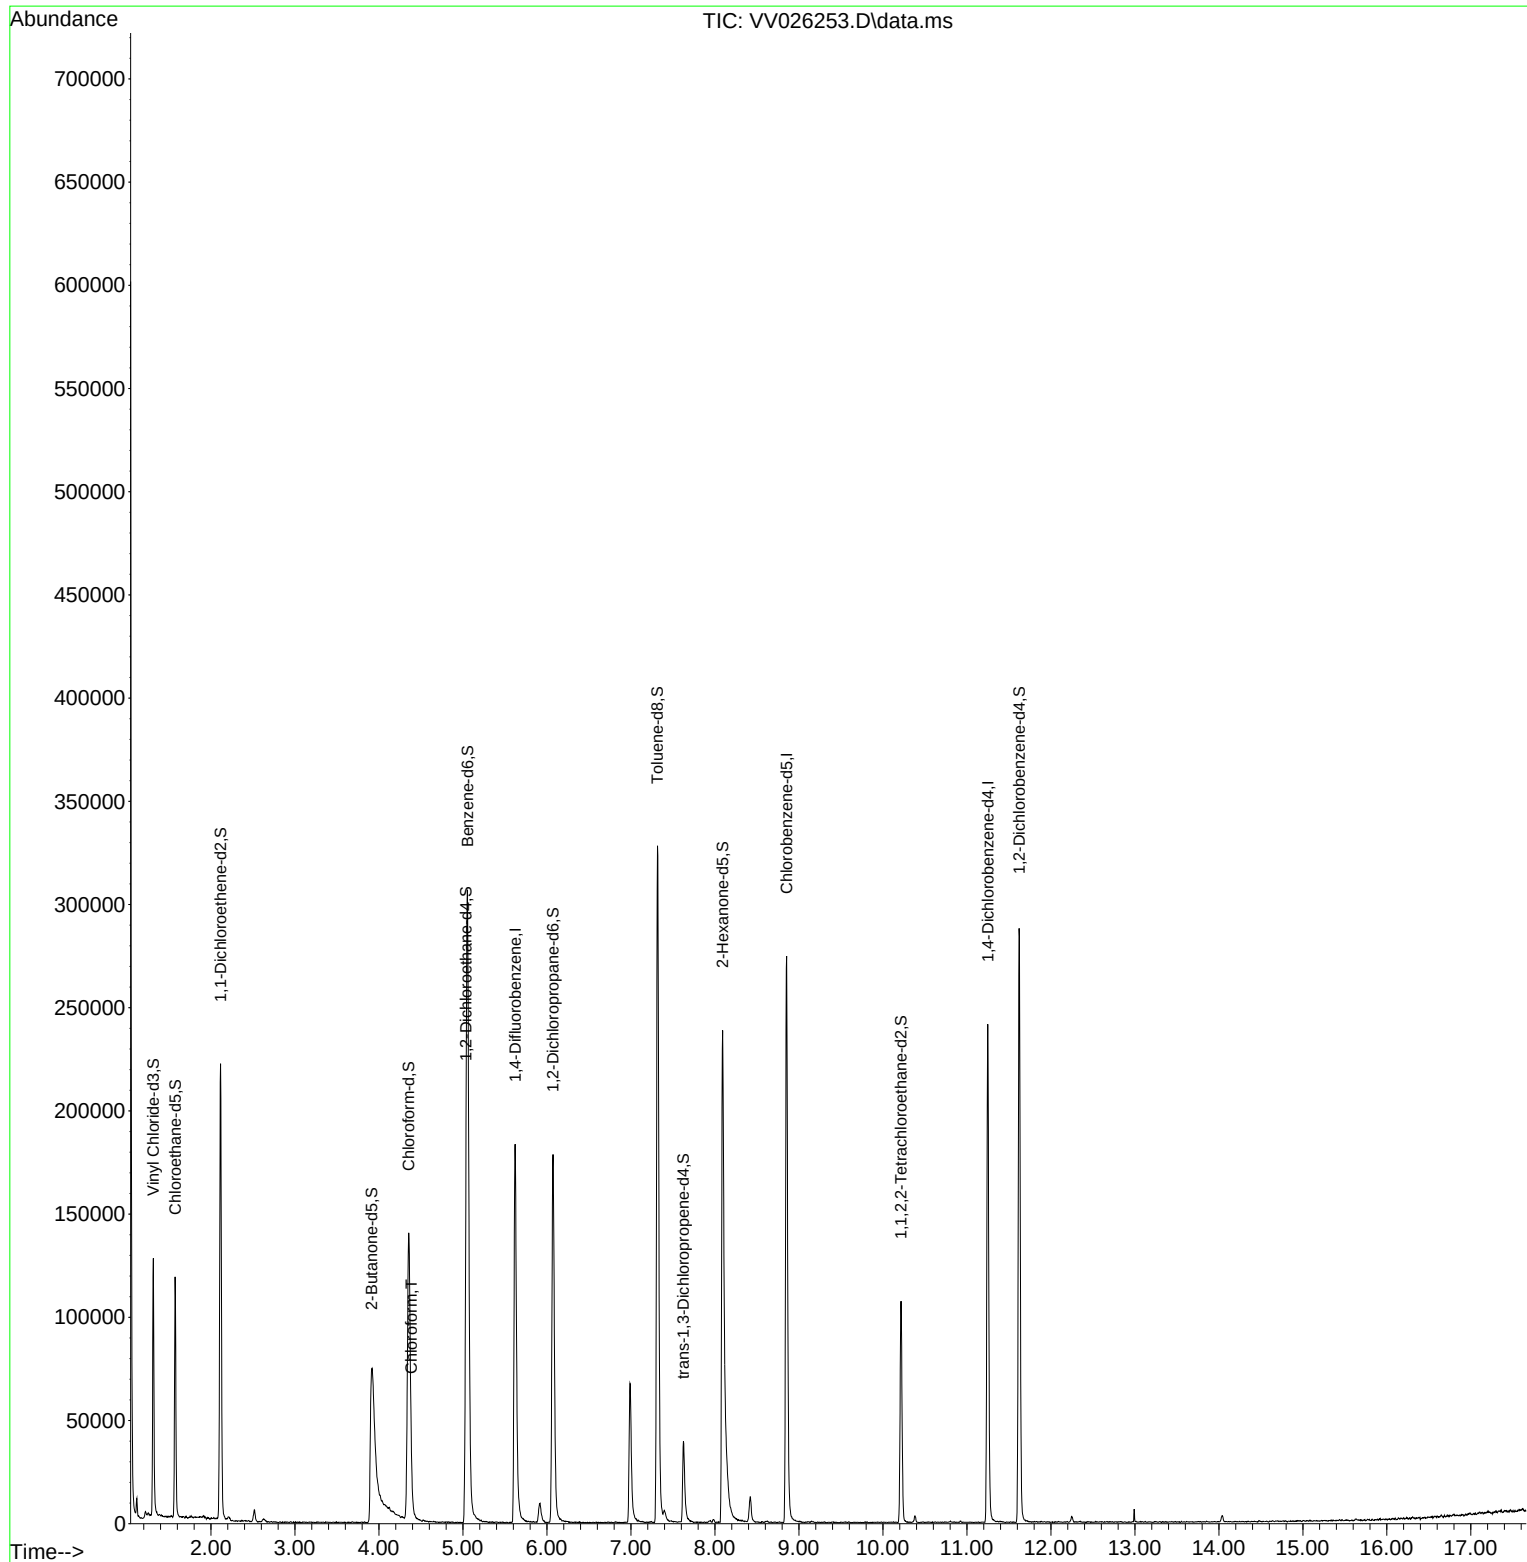

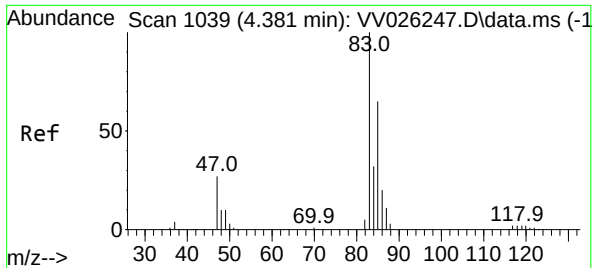

#25
Chloroform
Concen: 0.269 ug/L
RT: 4.384 min Scan# 10
Delta R.T. 0.003 min
Lab File: VV026253.D
Acq: 14 Jun 2022 23:00

Instrument :
MSVOA_V
ClientSampleId :
C0BD7

Tgt Ion: 83 Resp: 6477
Ion Ratio Lower Upper
83 100
85 70.2 45.3 84.1

