

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061422\
 Data File : VW026255.D
 Acq On : 14 Jun 2022 23:48
 Operator : SY/MD
 Sample : N3275-07 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD9

Quant Time: Jun 15 09:40:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 15 07:11:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	166894	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	159384	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	65366	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.314	65	83462	3.824	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.400%
7) Chloroethane-d5	1.574	69	73716	4.288	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.800%
11) 1,1-Dichloroethene-d2	2.114	63	115482	3.291	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.800%
20) 2-Butanone-d5	3.908	46	111577	68.525	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	137.060%#
24) Chloroform-d	4.355	84	149319	4.824	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.400%
26) 1,2-Dichloroethane-d4	5.037	65	65333	5.236	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.800%
32) Benzene-d6	5.053	84	290486	4.675	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%
36) 1,2-Dichloropropane-d6	6.072	67	91042	5.081	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.600%
41) Toluene-d8	7.317	98	228525	4.130	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.600%
43) trans-1,3-Dichloroprop...	7.625	79	25746	4.761	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.200%
46) 2-Hexanone-d5	8.092	63	93736	55.665	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.340%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	55858	5.232	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	76911	5.249	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.000%
Target Compounds					Qvalue	
25) Chloroform	4.388	83	6585	0.268	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026255.D
Acq On : 14 Jun 2022 23:48
Operator : SY/MD
Sample : N3275-07 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD9

Quant Time: Jun 15 09:40:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 15 07:11:20 2022
Response via : Initial Calibration

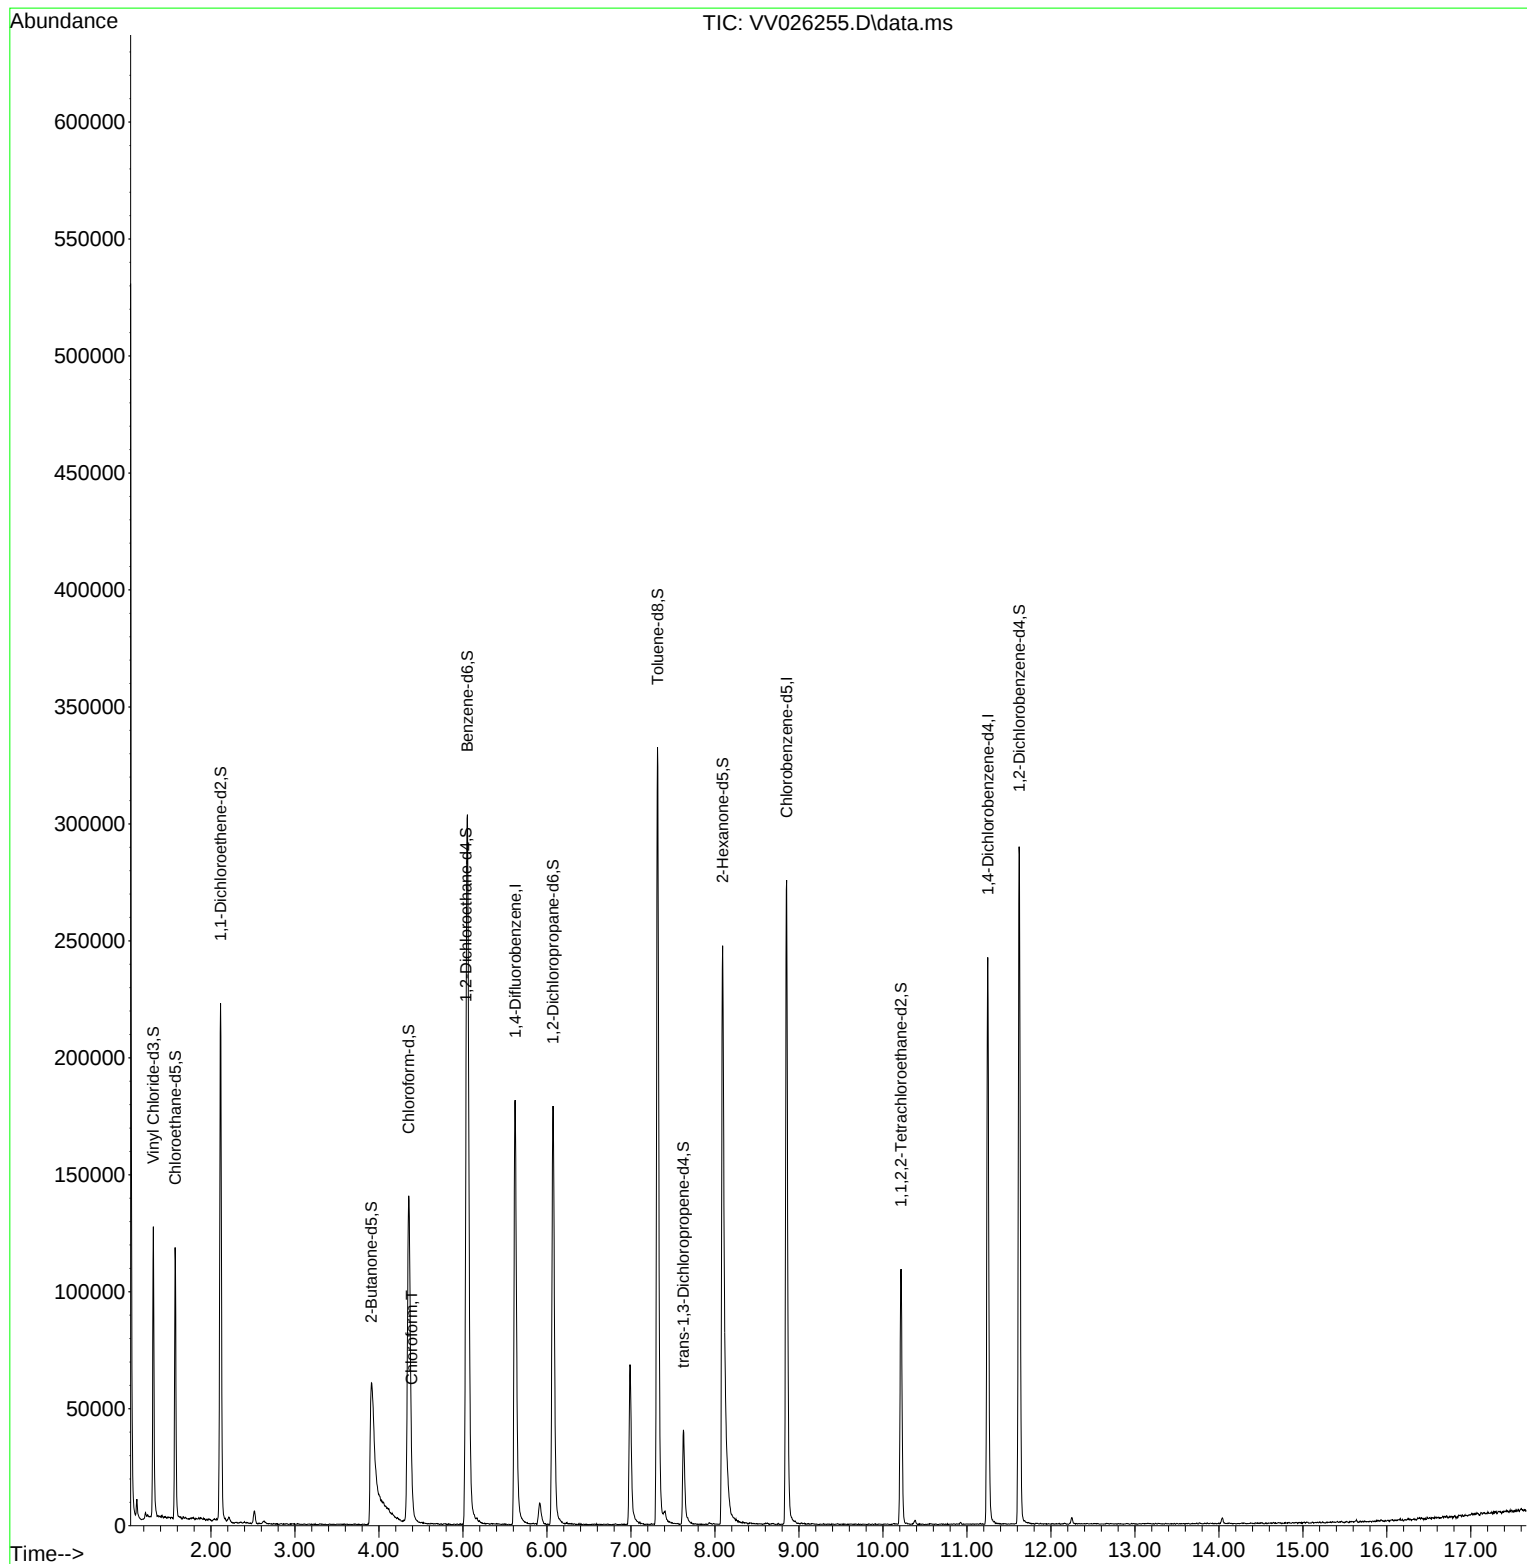

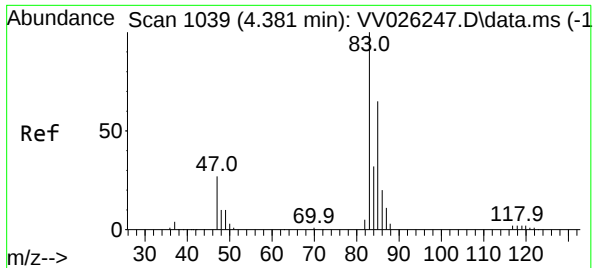

#25
 Chloroform
 Concen: 0.268 ug/L
 RT: 4.388 min Scan# 10
 Delta R.T. 0.007 min
 Lab File: VV026255.D
 Acq: 14 Jun 2022 23:48

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD9

Tgt Ion: 83 Resp: 6585
 Ion Ratio Lower Upper
 83 100
 85 60.3 45.3 84.1

