

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061422\
 Data File : VW026256.D
 Acq On : 15 Jun 2022 00:12
 Operator : SY/MD
 Sample : N3275-08 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBE0

Quant Time: Jun 15 09:40:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 15 07:11:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	158948	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	155377	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	64296	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.314	65	81866	3.938	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	78.800%	
7) Chloroethane-d5	1.574	69	73443	4.486	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	89.800%	
11) 1,1-Dichloroethene-d2	2.114	63	113072	3.383	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.600%	
20) 2-Butanone-d5	3.908	46	104602	67.453	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	134.900%#	
24) Chloroform-d	4.355	84	149326	5.066	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.400%	
26) 1,2-Dichloroethane-d4	5.040	65	65525	5.513	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	110.200%	
32) Benzene-d6	5.053	84	285833	4.719	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.400%	
36) 1,2-Dichloropropane-d6	6.072	67	90151	5.161	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	103.200%	
41) Toluene-d8	7.317	98	226375	4.197	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	84.000%	
43) trans-1,3-Dichloroprop...	7.625	79	24813	4.706	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	94.200%	
46) 2-Hexanone-d5	8.092	63	92212	56.172	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	112.340%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	54288	5.216	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	104.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	77295	5.363	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	107.200%	
Target Compounds						Qvalue
16) Methylene chloride	2.513	84	2588	0.207	ug/L	91
25) Chloroform	4.381	83	6189	0.265	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026256.D
Acq On : 15 Jun 2022 00:12
Operator : SY/MD
Sample : N3275-08 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE0

Quant Time: Jun 15 09:40:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 15 07:11:20 2022
Response via : Initial Calibration




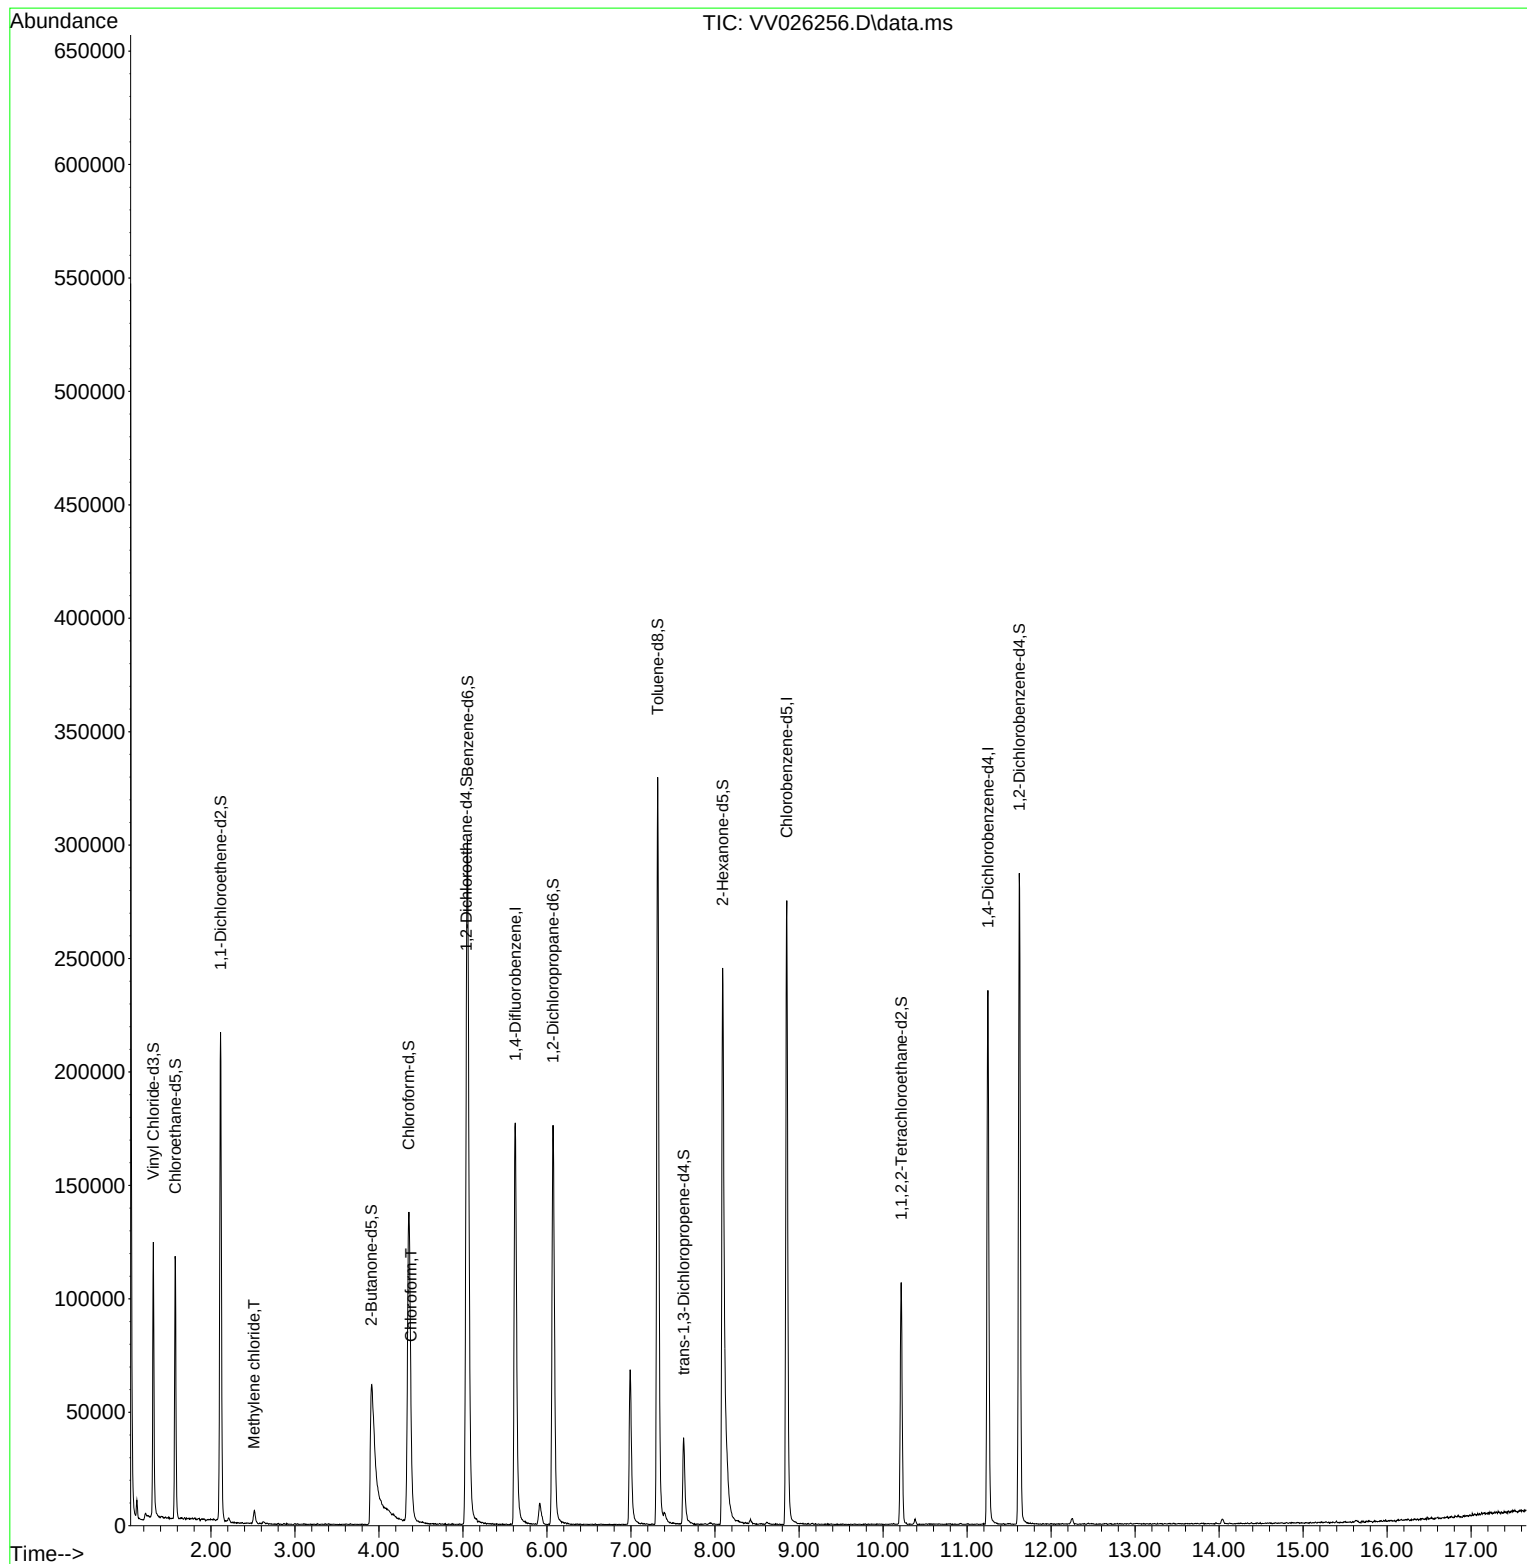


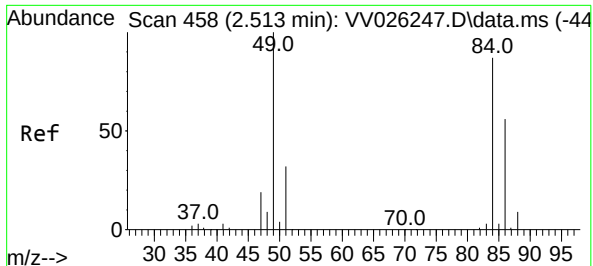

#16
Methylene chloride
Concen: 0.207 ug/L
RT: 2.513 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV026256.D
Acq: 15 Jun 2022 00:12

Instrument :
MSVOA_V
ClientSampleId :
COBE0

Tgt Ion: 84 Resp: 2588
Ion Ratio Lower Upper
84 100
86 60.9 45.1 83.7
49 104.5 82.3 152.9

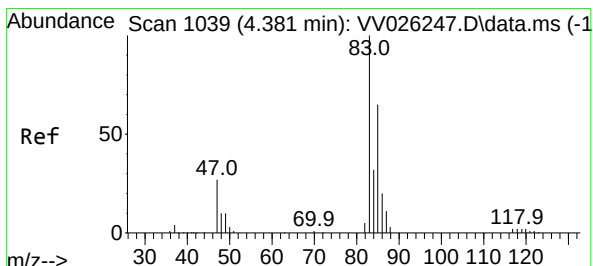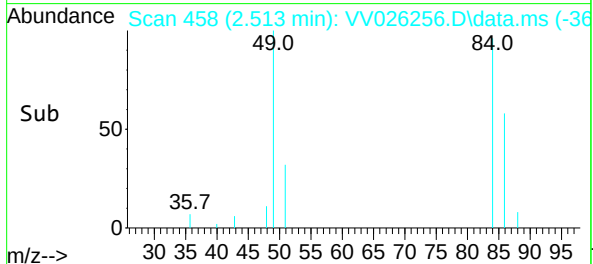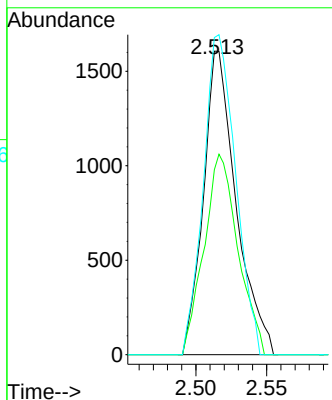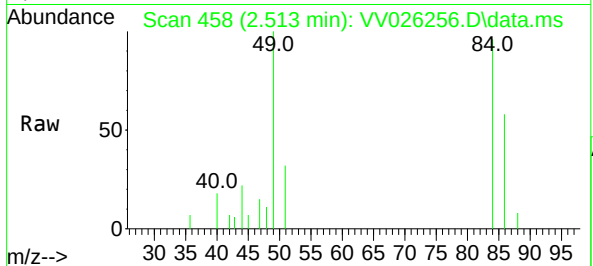

#25
Chloroform
Concen: 0.265 ug/L
RT: 4.381 min Scan# 1039
Delta R.T. 0.000 min
Lab File: VV026256.D
Acq: 15 Jun 2022 00:12

Tgt Ion: 83 Resp: 6189
Ion Ratio Lower Upper
83 100
85 67.7 45.3 84.1

