

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061422\
 Data File : VW026262.D
 Acq On : 15 Jun 2022 02:35
 Operator : SY/MD
 Sample : N3275-14 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE6

Quant Time: Jun 15 09:41:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 15 07:11:20 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	165835	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	162651	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	67694	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.314	65	82835	3.820	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	76.400%	
7) Chloroethane-d5	1.574	69	76043	4.452	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	89.000%	
11) 1,1-Dichloroethene-d2	2.114	63	115974	3.326	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	66.600%	
20) 2-Butanone-d5	3.912	46	118476	73.227	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	146.460%#	
24) Chloroform-d	4.355	84	153720	4.998	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.000%	
26) 1,2-Dichloroethane-d4	5.040	65	67812	5.469	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	109.400%	
32) Benzene-d6	5.053	84	303498	4.786	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.800%	
36) 1,2-Dichloropropane-d6	6.072	67	95631	5.230	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	104.600%	
41) Toluene-d8	7.317	98	236648	4.191	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	83.800%	
43) trans-1,3-Dichloroprop...	7.625	79	25924	4.697	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	94.000%	
46) 2-Hexanone-d5	8.092	63	96071	55.906	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	111.820%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	56814	5.215	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	104.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	82555	5.441	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	108.800%	
Target Compounds						
16) Methylene chloride	2.516	84	3639	0.278	ug/L	94
25) Chloroform	4.384	83	7901	0.324	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026262.D
Acq On : 15 Jun 2022 02:35
Operator : SY/MD
Sample : N3275-14 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE6

Quant Time: Jun 15 09:41:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 15 07:11:20 2022
Response via : Initial Calibration




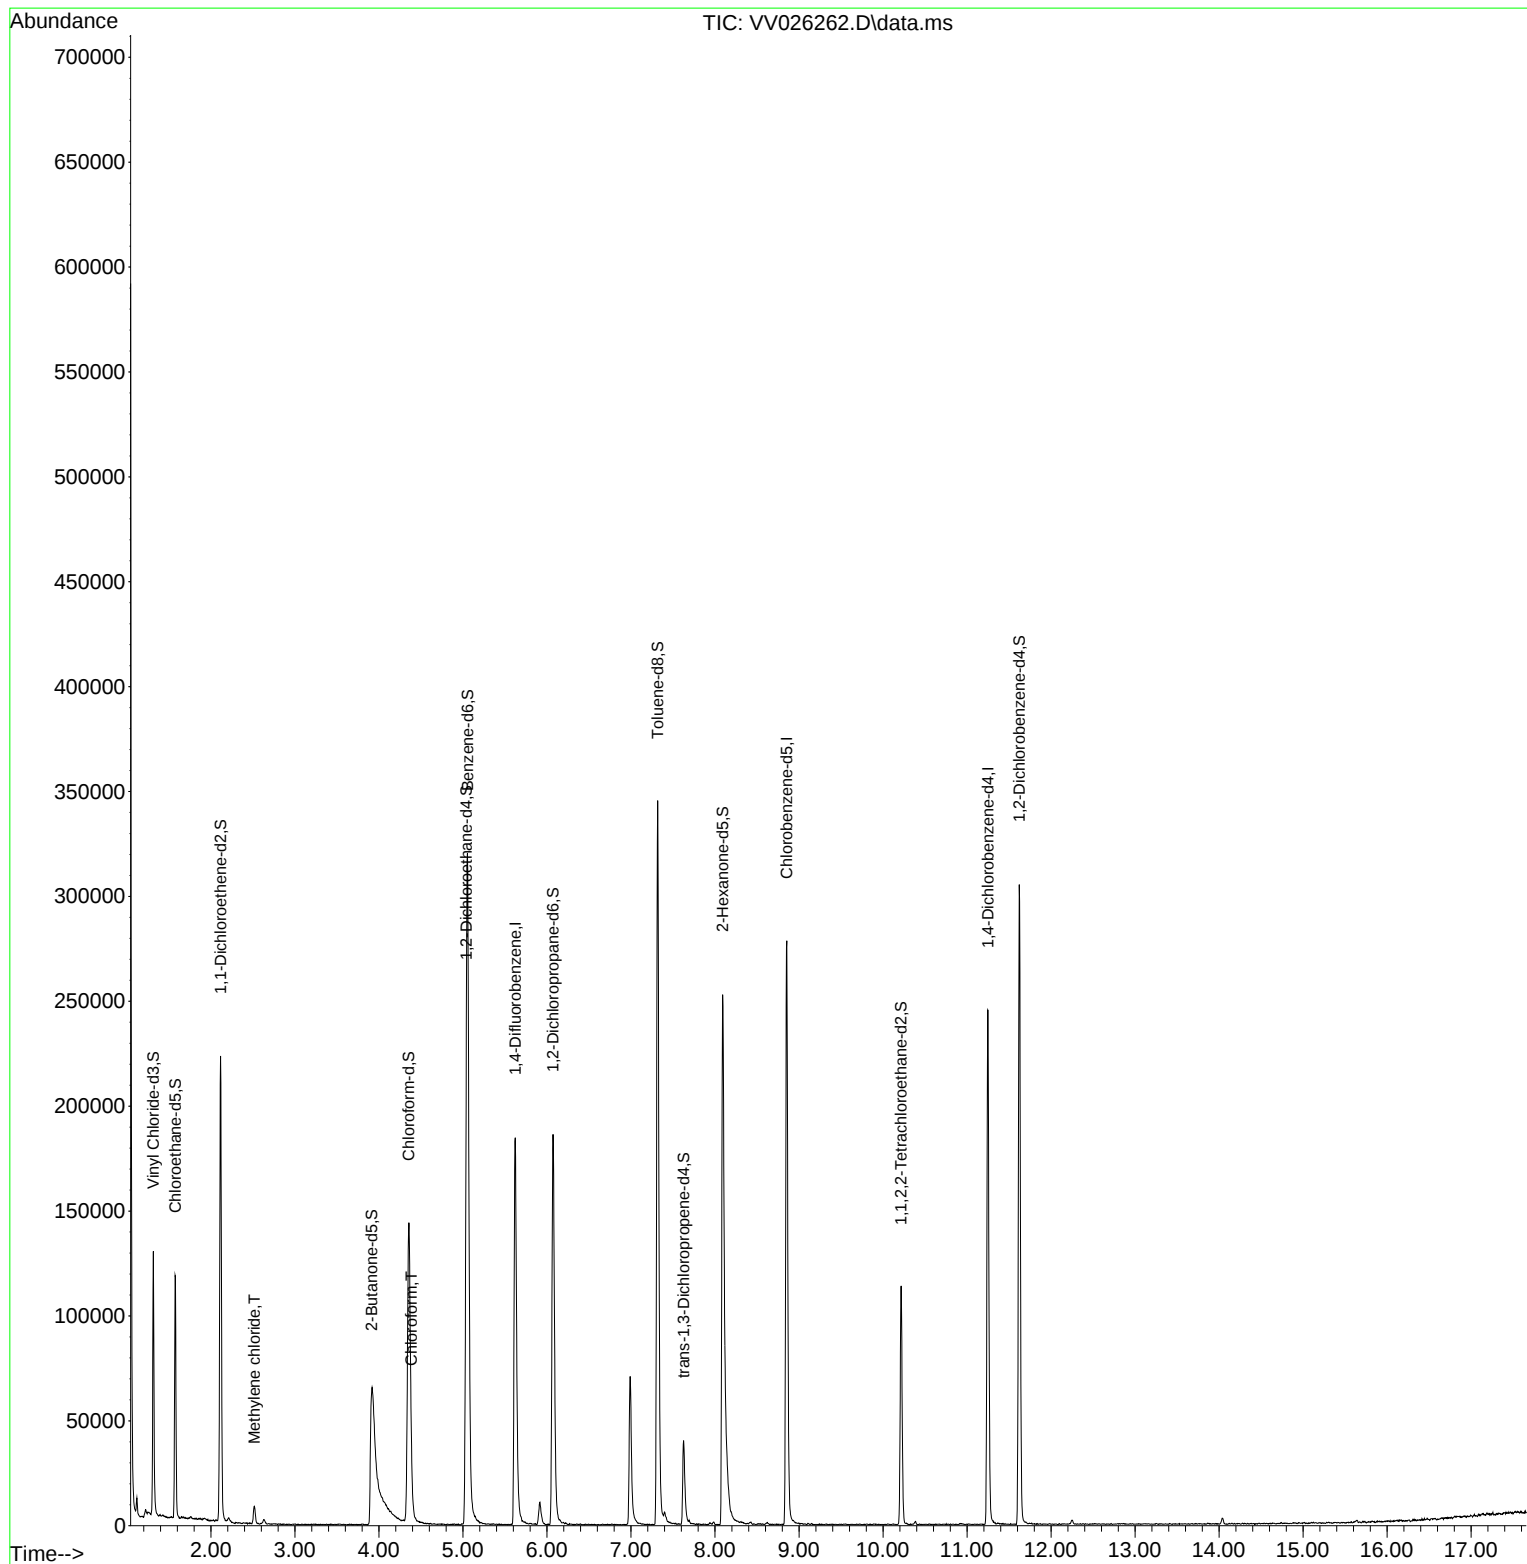


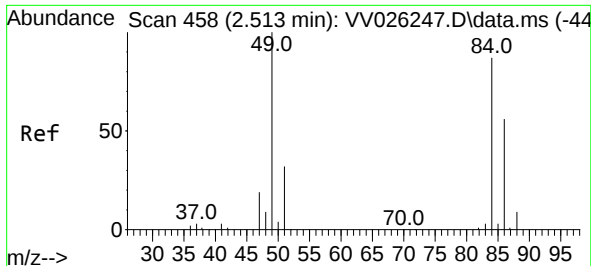

#16
Methylene chloride
Concen: 0.278 ug/L
RT: 2.516 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV026262.D
Acq: 15 Jun 2022 02:35

Instrument :
MSVOA_V
ClientSampleId :
C0BE6

Tgt Ion: 84 Resp: 3639
Ion Ratio Lower Upper
84 100
86 60.4 45.1 83.7
49 110.2 82.3 152.9

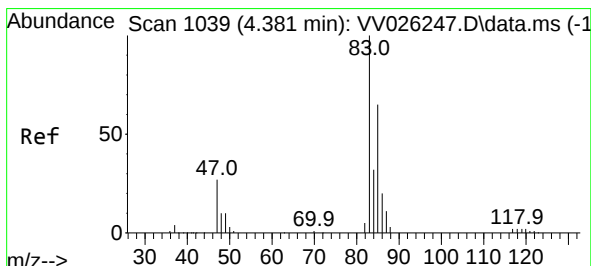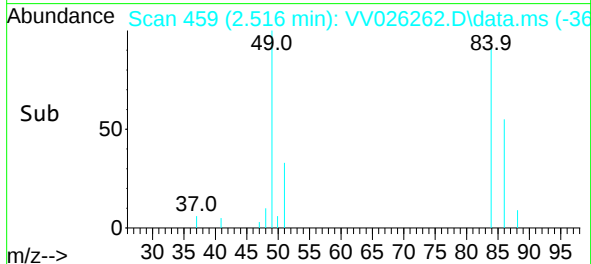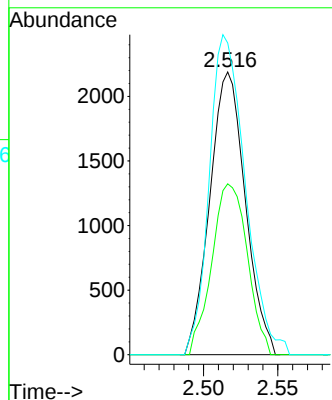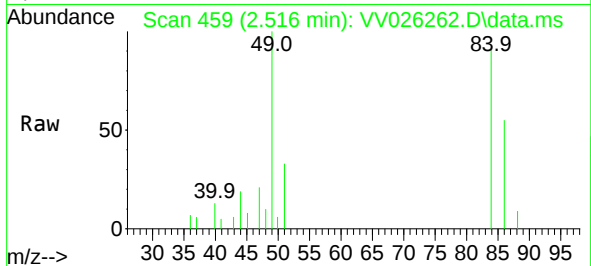

#25
Chloroform
Concen: 0.324 ug/L
RT: 4.384 min Scan# 1040
Delta R.T. 0.003 min
Lab File: VV026262.D
Acq: 15 Jun 2022 02:35

Tgt Ion: 83 Resp: 7901
Ion Ratio Lower Upper
83 100
85 63.0 45.3 84.1

