

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026225.D
 Acq On : 14 Jun 2022 10:29
 Operator : SY/MD
 Sample : VV0614WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK371

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026225.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.314	77	85	103	rVB	142520	155596	19.93%	2.826%
2	1.574	158	166	181	rVB	124930	142129	18.21%	2.582%
3	2.111	323	333	354	rVB	244479	354117	45.36%	6.432%
4	2.513	448	458	473	rVB	10418	17736	2.27%	0.322%
5	3.047	611	624	637	rBV4	5692	11850	1.52%	0.215%
6	3.905	880	891	925	rBV	41665	160971	20.62%	2.924%
7	4.352	1013	1030	1062	rBV2	140642	359152	46.01%	6.524%
8	5.050	1227	1247	1281	rBV2	312111	780610	100.00%	14.179%
9	5.616	1412	1423	1447	rBV	180578	373275	47.82%	6.780%
10	5.908	1498	1514	1530	rBV5	10755	22934	2.94%	0.417%
11	6.069	1550	1564	1588	rBV	177518	375389	48.09%	6.818%
12	6.986	1839	1849	1878	rBV	70315	133645	17.12%	2.428%
13	7.314	1940	1951	1971	rBV	341801	609005	78.02%	11.062%
14	7.391	1972	1975	1987	rVB5	5393	9494	1.22%	0.172%
15	7.622	2038	2047	2069	rBV	40733	72753	9.32%	1.321%
16	8.088	2182	2192	2230	rBV2	208201	490624	62.85%	8.912%
17	8.850	2417	2429	2456	rBV	274901	453634	58.11%	8.240%
18	10.214	2836	2853	2870	rBV	99293	160681	20.58%	2.919%
19	11.246	3163	3174	3190	rBV	239862	368768	47.24%	6.698%
20	11.622	3279	3291	3313	rBV	288375	453087	58.04%	8.230%




Sum of corrected areas: 5505450

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026225.D
Acq On : 14 Jun 2022 10:29
Operator : SY/MD
Sample : VV0614WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK371

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

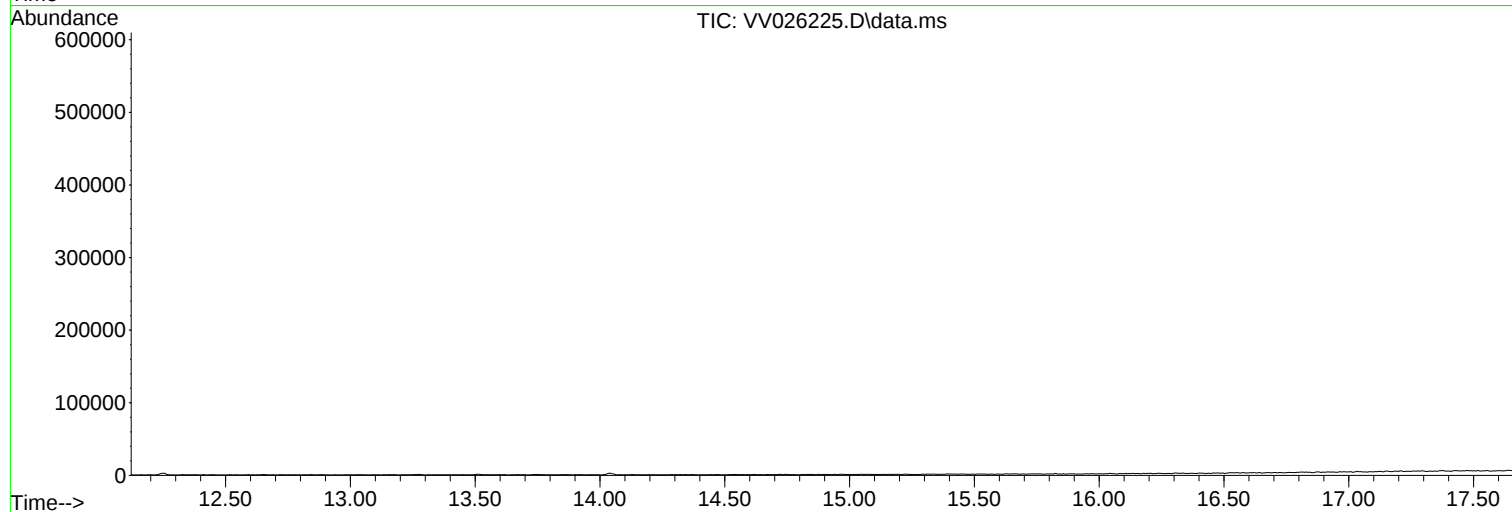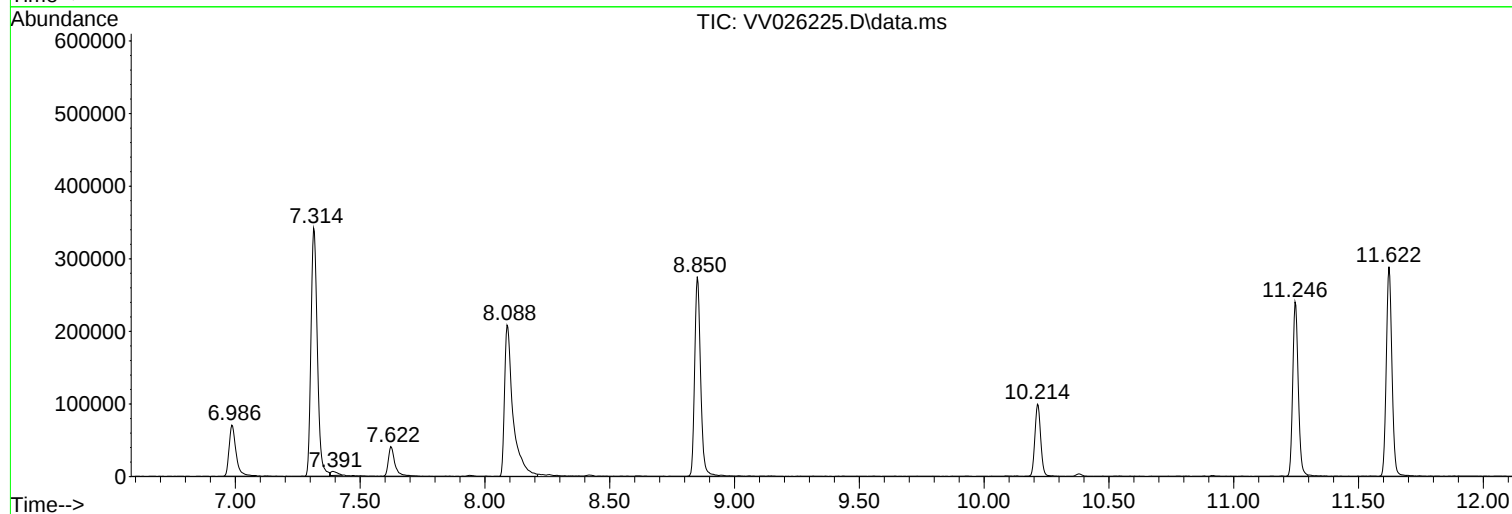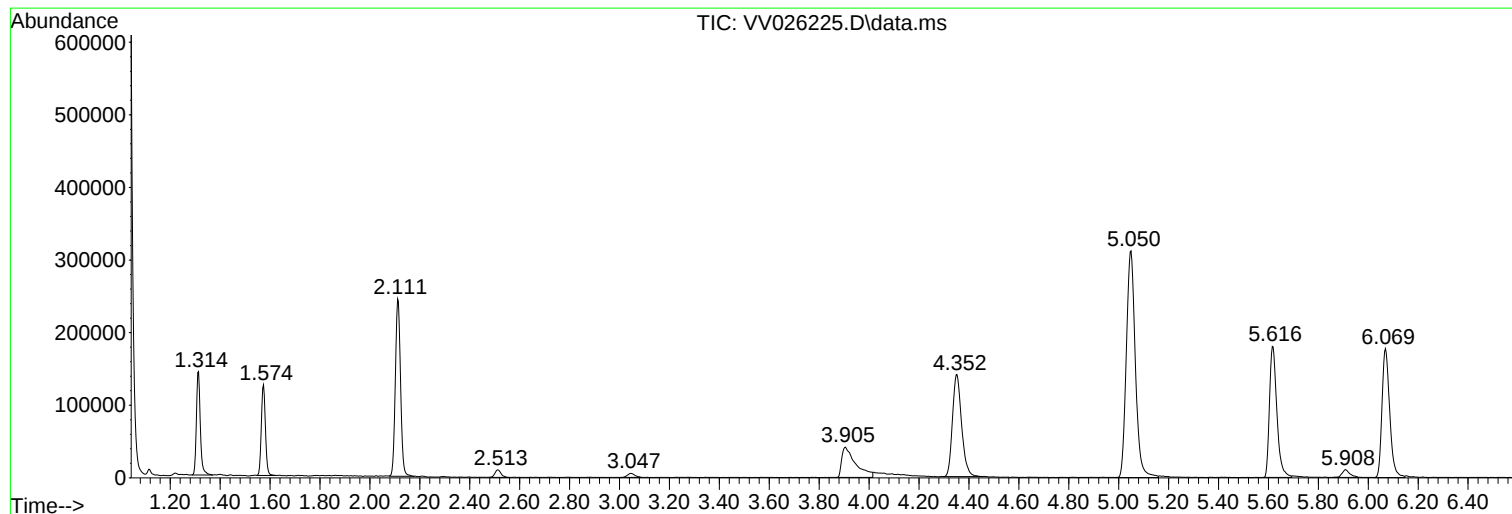

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026225.D
Acq On : 14 Jun 2022 10:29
Operator : SY/MD
Sample : VV0614WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK371

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026225.D
Acq On : 14 Jun 2022 10:29
Operator : SY/MD
Sample : VV0614WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK371

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
