

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026229.D
 Acq On : 14 Jun 2022 12:09
 Operator : SY/MD
 Sample : N3273-15
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B90

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026229.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	75	84	96	rBV	134789	160445	1.72%	0.966%
2	1.571	157	165	179	rBV	104413	120728	1.30%	0.727%
3	1.712	199	209	216	rBV	794665	954349	10.24%	5.745%
4	1.757	216	223	243	rVB	679351	895073	9.61%	5.388%
5	2.111	323	333	348	rBV	193106	281385	3.02%	1.694%
6	3.915	880	894	933	rBV3	131055	398084	4.27%	2.396%
7	4.355	1015	1031	1060	rBV2	123949	346650	3.72%	2.087%
8	5.050	1231	1247	1282	rBV2	252285	636217	6.83%	3.830%
9	5.619	1412	1424	1454	rBV	167379	345355	3.71%	2.079%
10	5.915	1503	1516	1549	rBV	302005	611212	6.56%	3.679%
11	6.072	1551	1565	1594	rVV	149650	303249	3.26%	1.825%
12	6.989	1840	1850	1877	rBV2	49720	99823	1.07%	0.601%
13	7.317	1940	1952	1972	rBV	260864	458571	4.92%	2.760%
14	7.976	2136	2157	2184	rBV	5660853	9316177	100.00%	56.078%
15	8.092	2184	2193	2226	rVB2	197780	431303	4.63%	2.596%
16	8.854	2418	2430	2456	rBV	247672	448284	4.81%	2.698%
17	10.217	2843	2854	2873	rBV	84791	133954	1.44%	0.806%
18	11.249	3164	3175	3195	rBV	211835	324386	3.48%	1.953%
19	11.622	3281	3291	3309	rVB	222437	347654	3.73%	2.093%




Sum of corrected areas: 16612899

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026229.D
Acq On : 14 Jun 2022 12:09
Operator : SY/MD
Sample : N3273-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

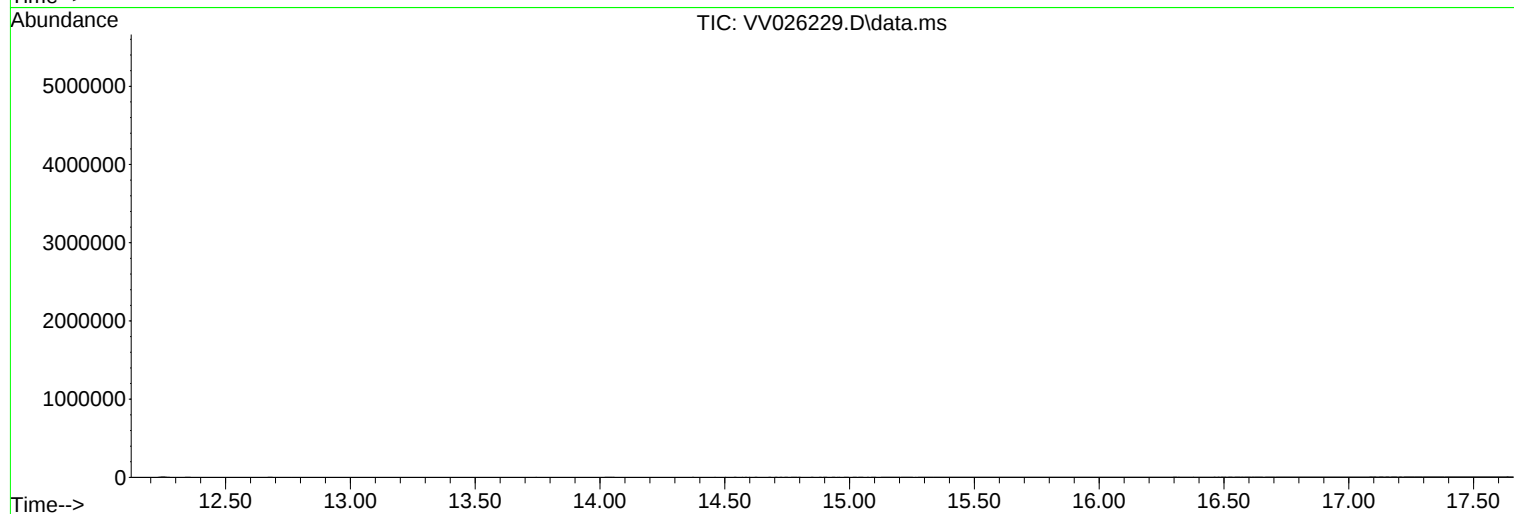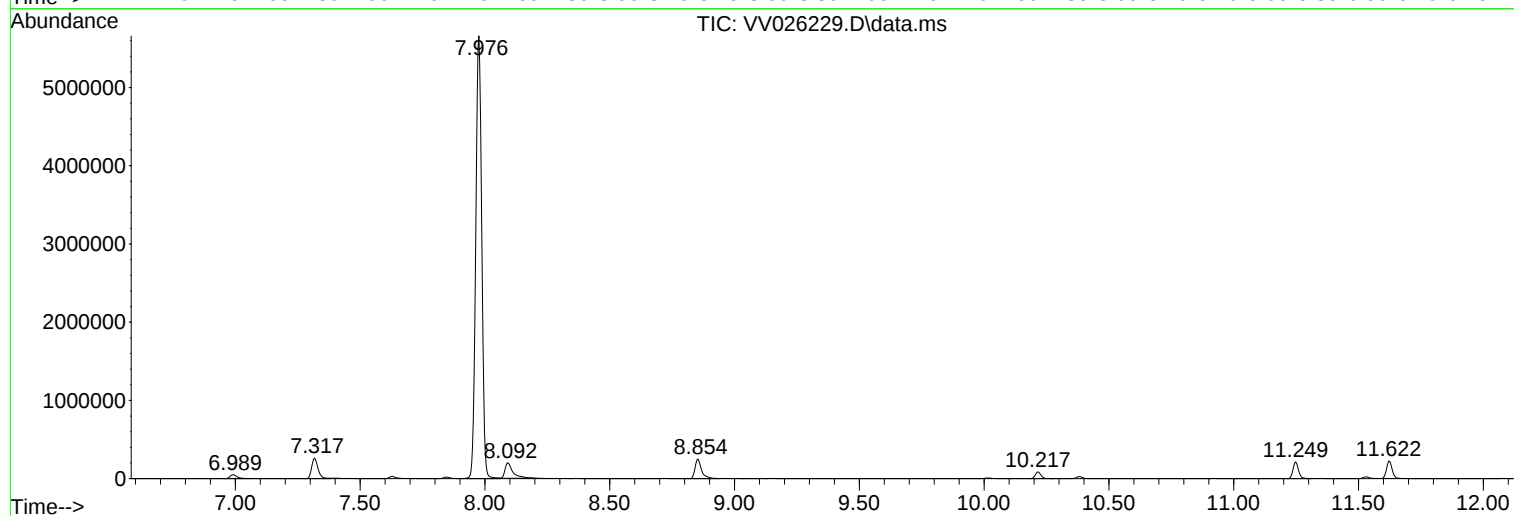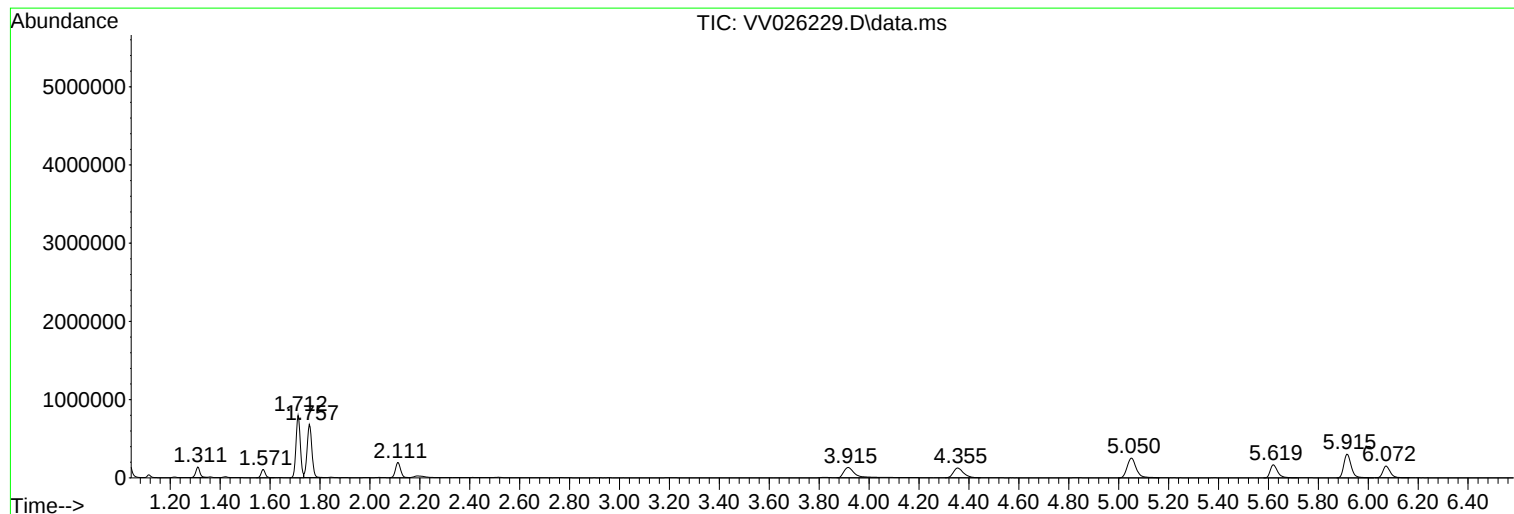

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026229.D
Acq On : 14 Jun 2022 12:09
Operator : SY/MD
Sample : N3273-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026229.D
Acq On : 14 Jun 2022 12:09
Operator : SY/MD
Sample : N3273-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc