

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026232.D
 Acq On : 14 Jun 2022 13:20
 Operator : SY/MD
 Sample : N3312-18
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.117	19	24	33	rVB	7811	8201	1.04%	0.144%
2	1.314	77	85	106	rBV	138031	150103	19.00%	2.638%
3	1.574	159	166	181	rVB	126099	141869	17.96%	2.493%
4	2.114	323	334	356	rVB	240815	345493	43.73%	6.072%
5	2.516	449	459	473	rBV2	15294	25655	3.25%	0.451%
6	3.912	882	893	922	rBV	46546	173965	22.02%	3.057%
7	4.355	1015	1031	1064	rVB	142312	362497	45.88%	6.371%
8	5.053	1232	1248	1280	rBV2	318031	790020	100.00%	13.884%
9	5.622	1412	1425	1450	rBV	187959	384704	48.70%	6.761%
10	5.921	1503	1518	1536	rVB8	10976	27465	3.48%	0.483%
11	6.072	1552	1565	1591	rBV	182701	376499	47.66%	6.617%
12	6.989	1840	1850	1876	rBV	71111	137561	17.41%	2.417%
13	7.317	1941	1952	1973	rBV	339586	604787	76.55%	10.629%
14	7.625	2036	2048	2067	rBV	42695	76896	9.73%	1.351%
15	8.091	2183	2193	2241	rBV2	245615	572076	72.41%	10.054%
16	8.853	2415	2430	2451	rBV	286282	474026	60.00%	8.331%
17	10.217	2837	2854	2871	rBV	110672	175474	22.21%	3.084%
18	10.384	2895	2906	2915	rVB3	6151	9881	1.25%	0.174%
19	11.249	3164	3175	3198	rBV	249731	385906	48.85%	6.782%
20	11.625	3277	3292	3309	rBV	297271	467155	59.13%	8.210%




Sum of corrected areas: 5690233

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026232.D
Acq On : 14 Jun 2022 13:20
Operator : SY/MD
Sample : N3312-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

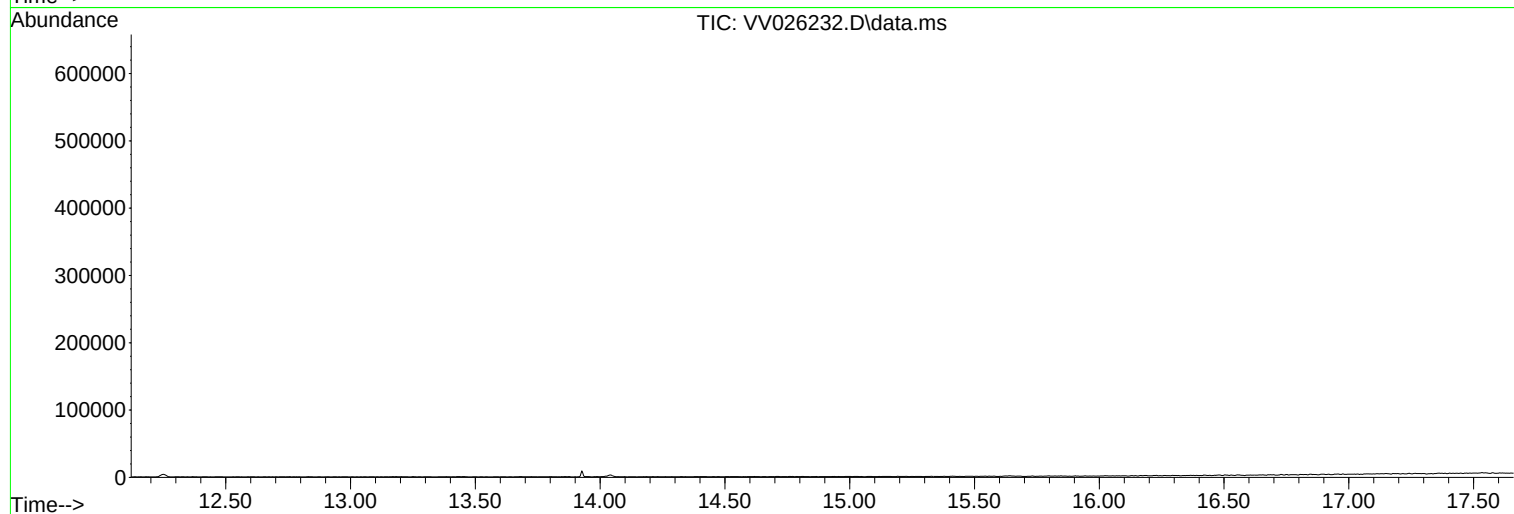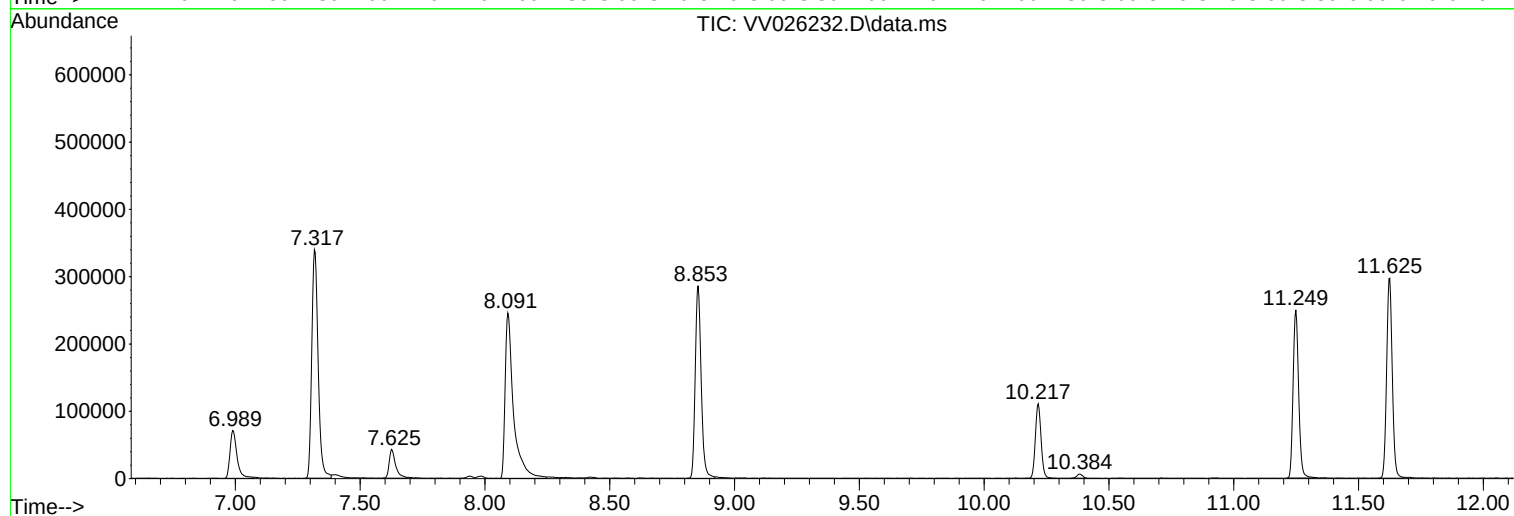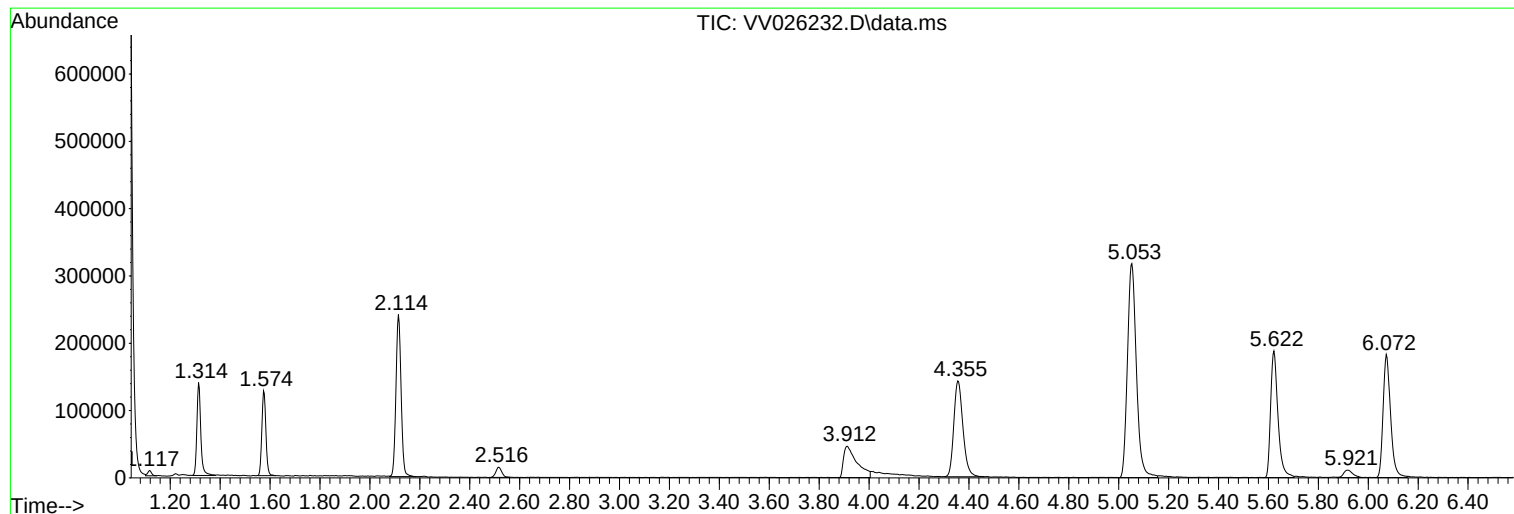

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026232.D
Acq On : 14 Jun 2022 13:20
Operator : SY/MD
Sample : N3312-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026232.D
Acq On : 14 Jun 2022 13:20
Operator : SY/MD
Sample : N3312-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
