

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026233.D
 Acq On : 14 Jun 2022 13:44
 Operator : SY/MD
 Sample : N3272-13DL2 8000X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B57DL2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026233.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.117	19	24	37	rVB3	9004	9633	1.22%	0.150%
2	1.314	77	85	101	rBV	140198	149794	19.02%	2.325%
3	1.574	158	166	182	rBV	125571	145174	18.43%	2.254%
4	2.114	323	334	353	rVB	245232	349782	44.41%	5.430%
5	2.516	445	459	471	rBV	11639	18001	2.29%	0.279%
6	3.915	884	894	936	rBV2	44235	192642	24.46%	2.991%
7	4.355	1014	1031	1058	rBV	141621	360454	45.76%	5.596%
8	5.053	1230	1248	1277	rBV2	319232	787663	100.00%	12.228%
9	5.622	1413	1425	1452	rBV	187198	388831	49.37%	6.036%
10	5.918	1503	1517	1552	rBV	333321	677067	85.96%	10.511%
11	6.072	1552	1565	1588	rBV	181800	377047	47.87%	5.853%
12	6.989	1839	1850	1876	rBV	71406	141667	17.99%	2.199%
13	7.317	1938	1952	1973	rBV	350086	621024	78.84%	9.641%
14	7.397	1974	1977	1995	rVB2	5695	10740	1.36%	0.167%
15	7.625	2038	2048	2068	rBV2	40647	77430	9.83%	1.202%
16	7.979	2150	2158	2170	rVB4	8453	14926	1.89%	0.232%
17	8.091	2182	2193	2227	rBV2	252382	568351	72.16%	8.823%
18	8.854	2414	2430	2448	rBV	291724	481982	61.19%	7.482%
19	10.217	2840	2854	2875	rBV	114527	181745	23.07%	2.821%
20	11.249	3163	3175	3196	rBV	265351	403399	51.21%	6.262%
21	11.622	3279	3291	3313	rBV	305041	484200	61.47%	7.517%




Sum of corrected areas: 6441552

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026233.D
Acq On : 14 Jun 2022 13:44
Operator : SY/MD
Sample : N3272-13DL2 8000X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B57DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

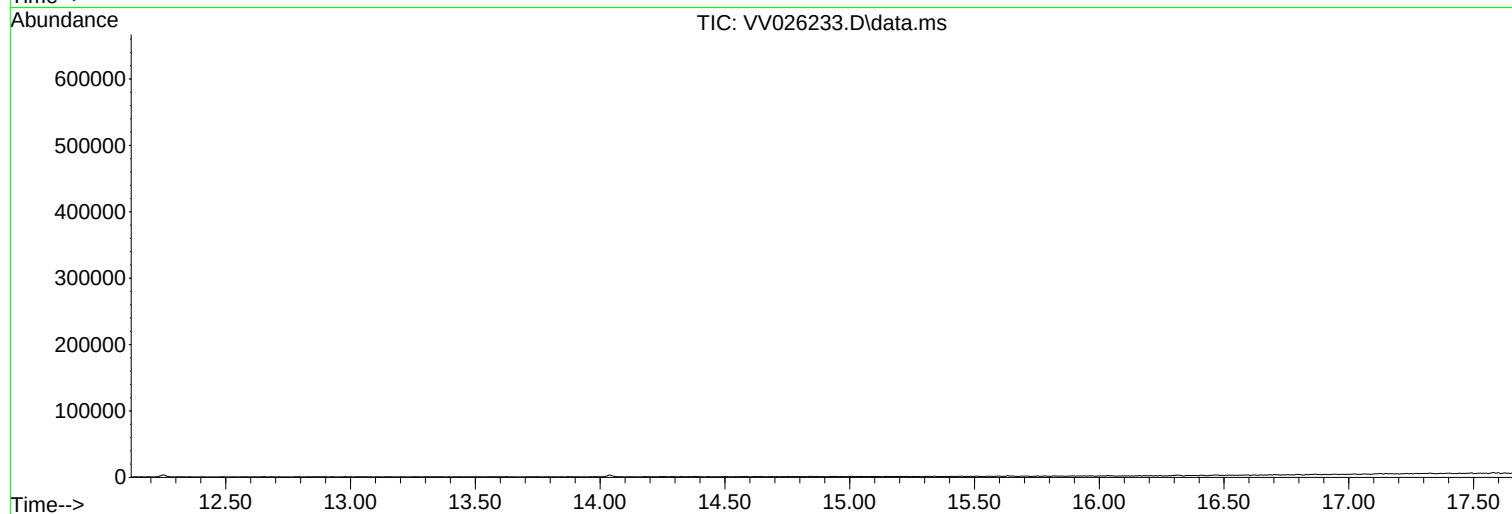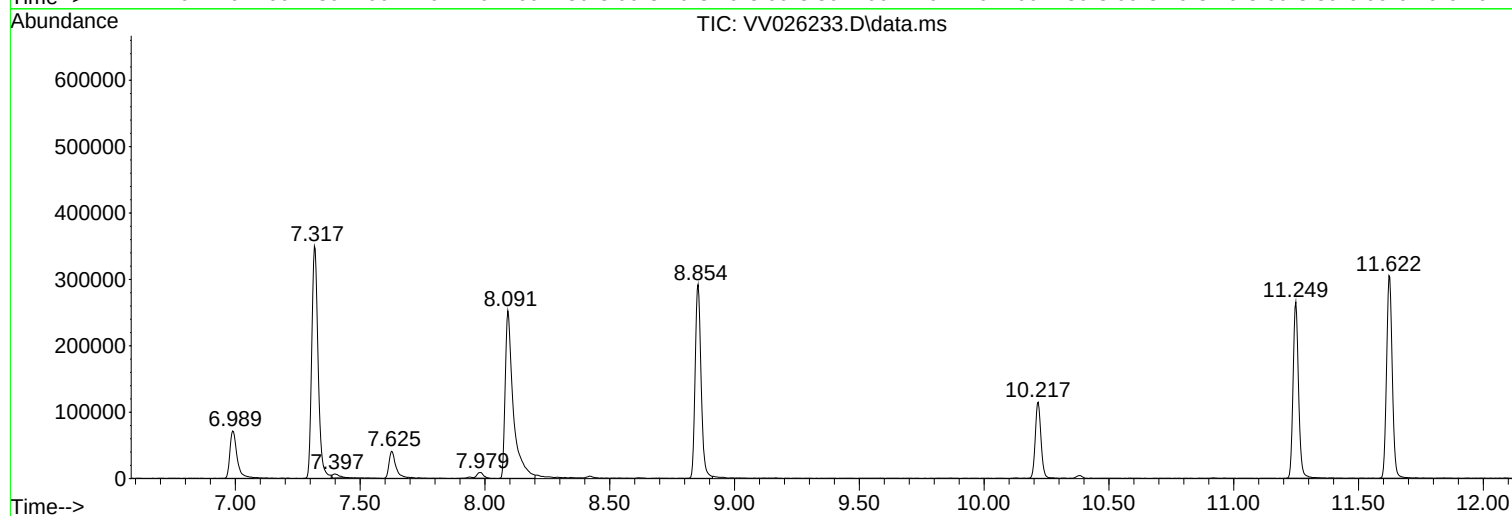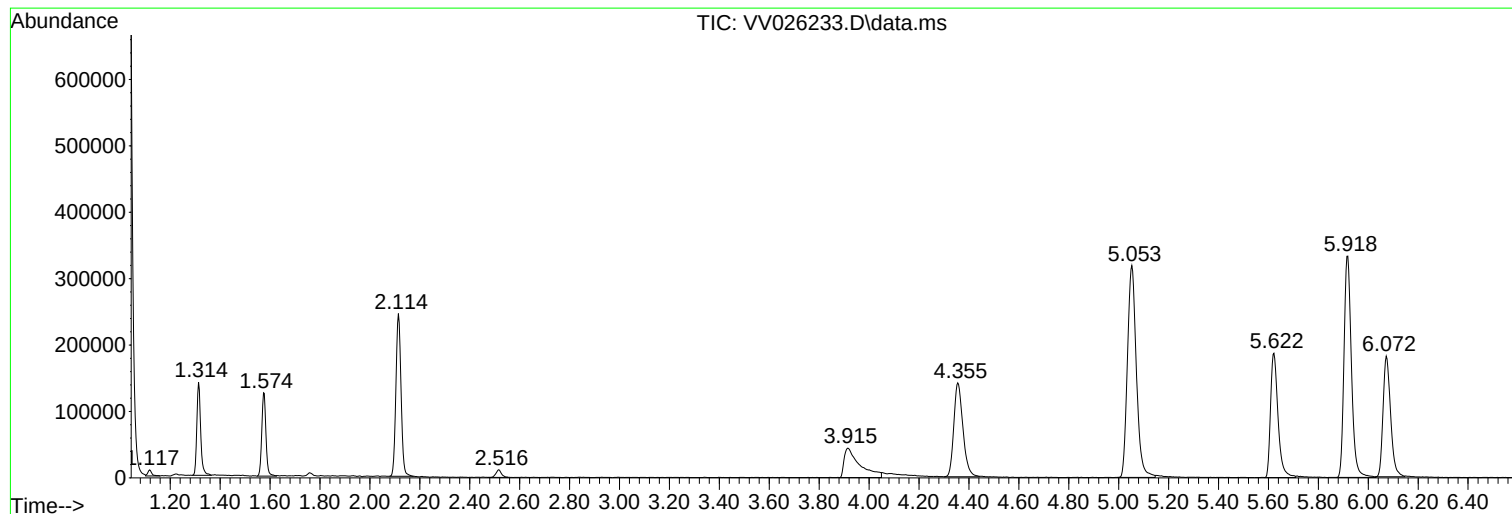

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026233.D
Acq On : 14 Jun 2022 13:44
Operator : SY/MD
Sample : N3272-13DL2 8000X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B57DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026233.D
Acq On : 14 Jun 2022 13:44
Operator : SY/MD
Sample : N3272-13DL2 8000X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B57DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc