

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026234.D
 Acq On : 14 Jun 2022 14:08
 Operator : SY/MD
 Sample : N3277-05DL 400X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BA4DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026234.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.314	78	85	98	rVB	53210	56062	6.70%	1.082%
2	1.574	158	166	177	rBV	78968	89677	10.71%	1.731%
3	2.114	324	334	352	rVB	105421	152442	18.21%	2.943%
4	2.516	449	459	470	rBV	11356	18065	2.16%	0.349%
5	3.925	879	897	949	rBV3	57921	304995	36.44%	5.887%
6	4.359	1017	1032	1057	rBV	102197	261763	31.28%	5.053%
7	5.053	1232	1248	1274	rBV2	198018	501664	59.94%	9.684%
8	5.622	1413	1425	1447	rBV	187787	383267	45.79%	7.398%
9	5.915	1504	1516	1542	rBV	415906	836963	100.00%	16.156%
10	6.072	1553	1565	1586	rBV2	132316	273387	32.66%	5.277%
11	6.992	1838	1851	1870	rBV	33630	65426	7.82%	1.263%
12	7.320	1942	1953	1978	rBV	177229	318857	38.10%	6.155%
13	7.629	2039	2049	2076	rBV2	18970	37866	4.52%	0.731%
14	7.982	2151	2159	2172	rVB4	6535	10850	1.30%	0.209%
15	8.092	2180	2193	2236	rBV2	238905	528373	63.13%	10.199%
16	8.420	2285	2295	2306	rBV4	7100	12458	1.49%	0.240%
17	8.854	2419	2430	2456	rBV	289366	473833	56.61%	9.147%
18	10.217	2842	2854	2867	rBV	94499	148954	17.80%	2.875%
19	11.249	3163	3175	3197	rBV	242817	382824	45.74%	7.390%
20	11.622	3280	3291	3313	rBV	201364	322715	38.56%	6.229%




Sum of corrected areas: 5180441

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026234.D
Acq On : 14 Jun 2022 14:08
Operator : SY/MD
Sample : N3277-05DL 400X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BA4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

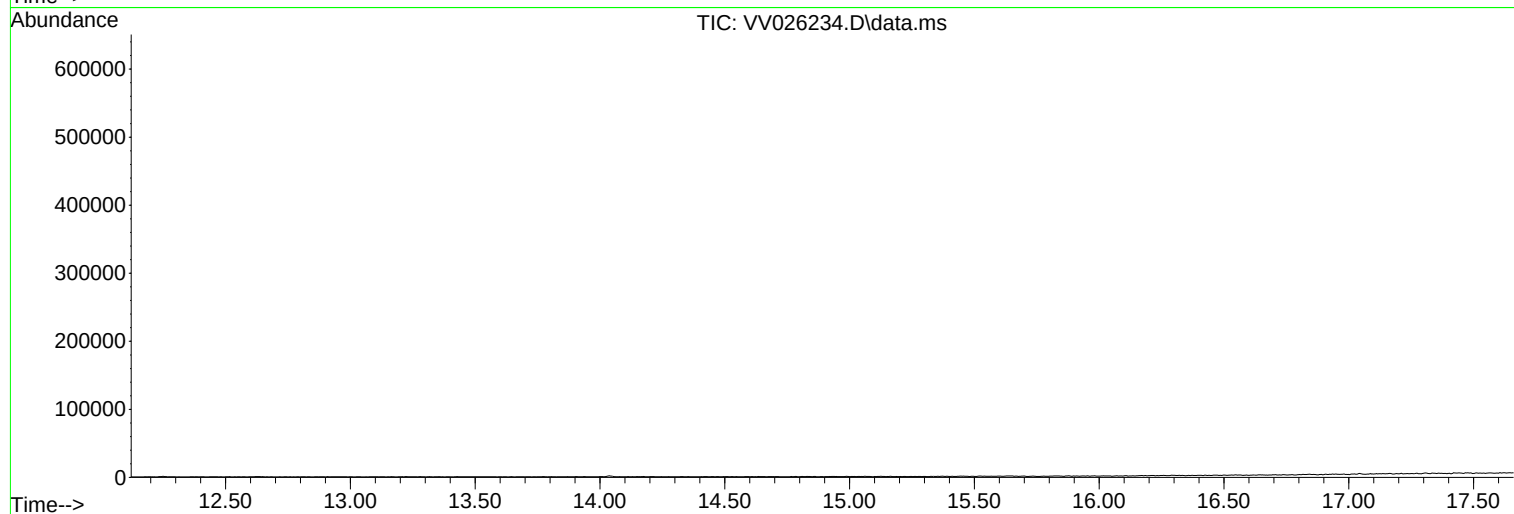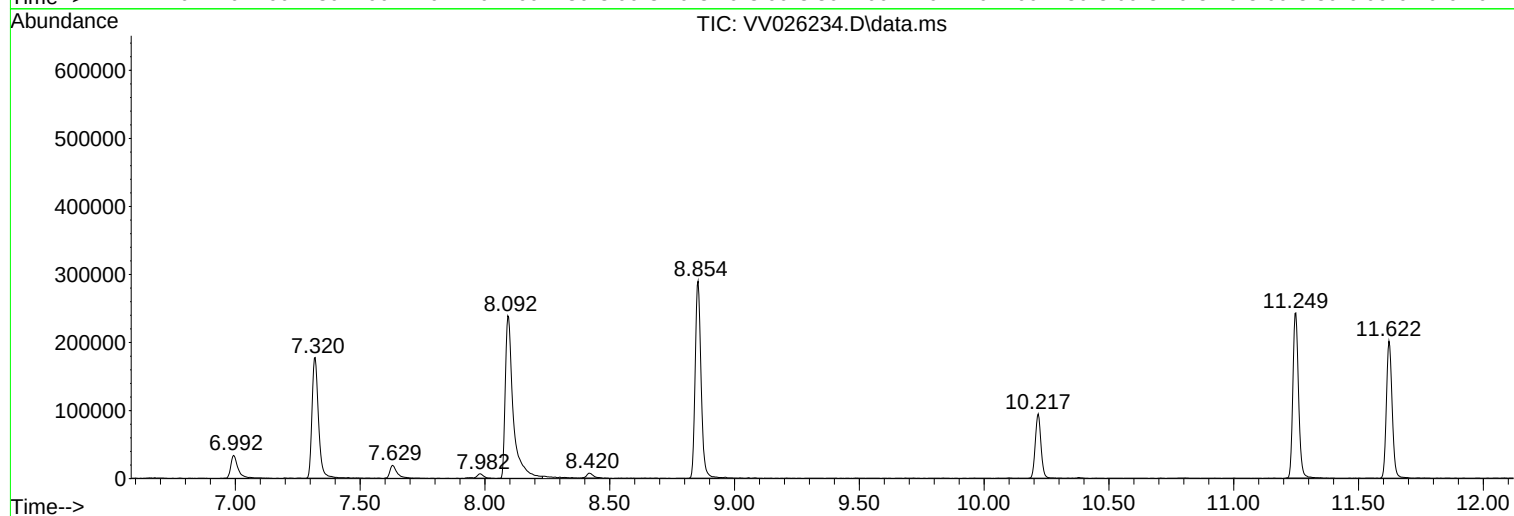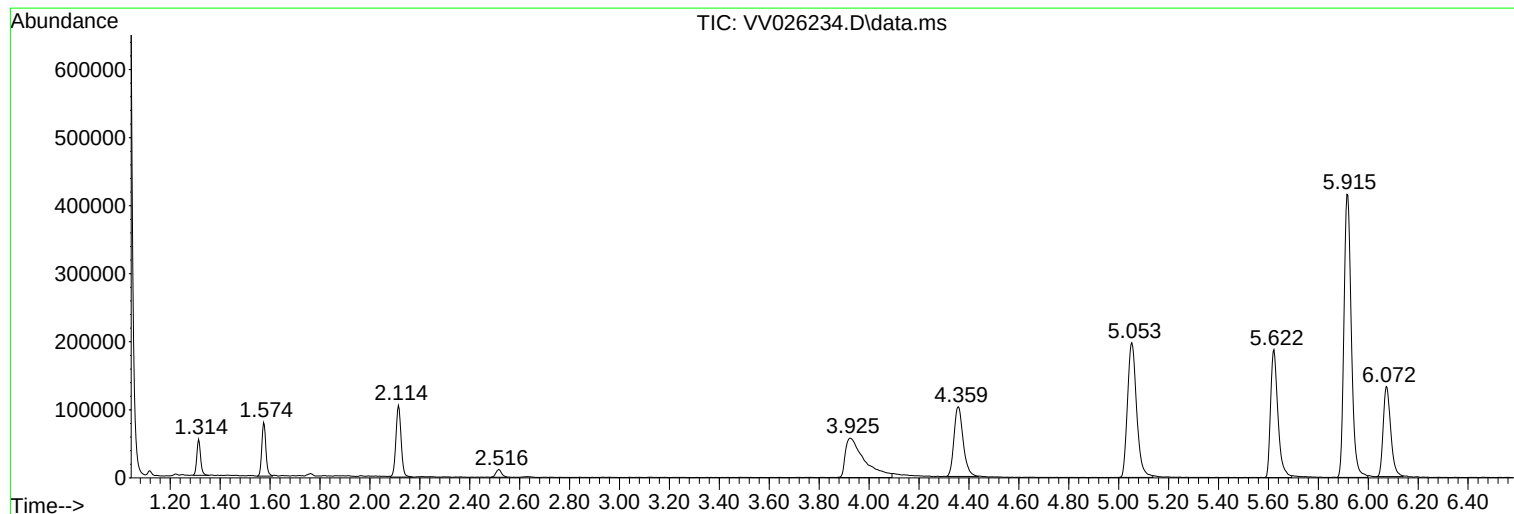

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026234.D
Acq On : 14 Jun 2022 14:08
Operator : SY/MD
Sample : N3277-05DL 400X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BA4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026234.D
Acq On : 14 Jun 2022 14:08
Operator : SY/MD
Sample : N3277-05DL 400X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BA4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc