

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026235.D
 Acq On : 14 Jun 2022 14:30
 Operator : SY/MD
 Sample : N3277-09 100X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BA8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026235.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	19	24	44	rVB3	9634	11572	2.18%	0.253%
2	1.220	48	56	62	rBV5	3839	5428	1.02%	0.119%
3	1.314	77	85	99	rVB	52041	56137	10.57%	1.228%
4	1.574	159	166	176	rBV	76208	88636	16.69%	1.938%
5	2.114	323	334	352	rVB	101188	148961	28.05%	3.257%
6	2.516	451	459	472	rVB	8473	13583	2.56%	0.297%
7	3.925	881	897	940	rBV4	59128	287371	54.12%	6.284%
8	4.359	1017	1032	1059	rVB2	102777	263342	49.59%	5.759%
9	5.056	1231	1249	1277	rBV2	200937	509762	95.99%	11.147%
10	5.625	1414	1426	1454	rBV	188843	392004	73.82%	8.572%
11	5.921	1505	1518	1552	rBV2	97557	208005	39.17%	4.549%
12	6.076	1552	1566	1594	rBV	135533	279264	52.59%	6.107%
13	6.995	1842	1852	1877	rBV	34029	66590	12.54%	1.456%
14	7.320	1941	1953	1980	rBV	174705	314705	59.26%	6.882%
15	7.632	2041	2050	2069	rBV	18536	35504	6.69%	0.776%
16	7.982	2150	2159	2176	rVB3	8442	14168	2.67%	0.310%
17	8.095	2184	2194	2232	rBV2	229740	531035	100.00%	11.613%
18	8.854	2419	2430	2451	rBV	296408	484965	91.32%	10.605%
19	10.217	2843	2854	2867	rBV	92818	147299	27.74%	3.221%
20	11.249	3164	3175	3200	rBV	249942	395025	74.39%	8.638%
21	11.625	3280	3292	3308	rBV	202181	319557	60.18%	6.988%




Sum of corrected areas: 4572913

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026235.D
Acq On : 14 Jun 2022 14:30
Operator : SY/MD
Sample : N3277-09 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

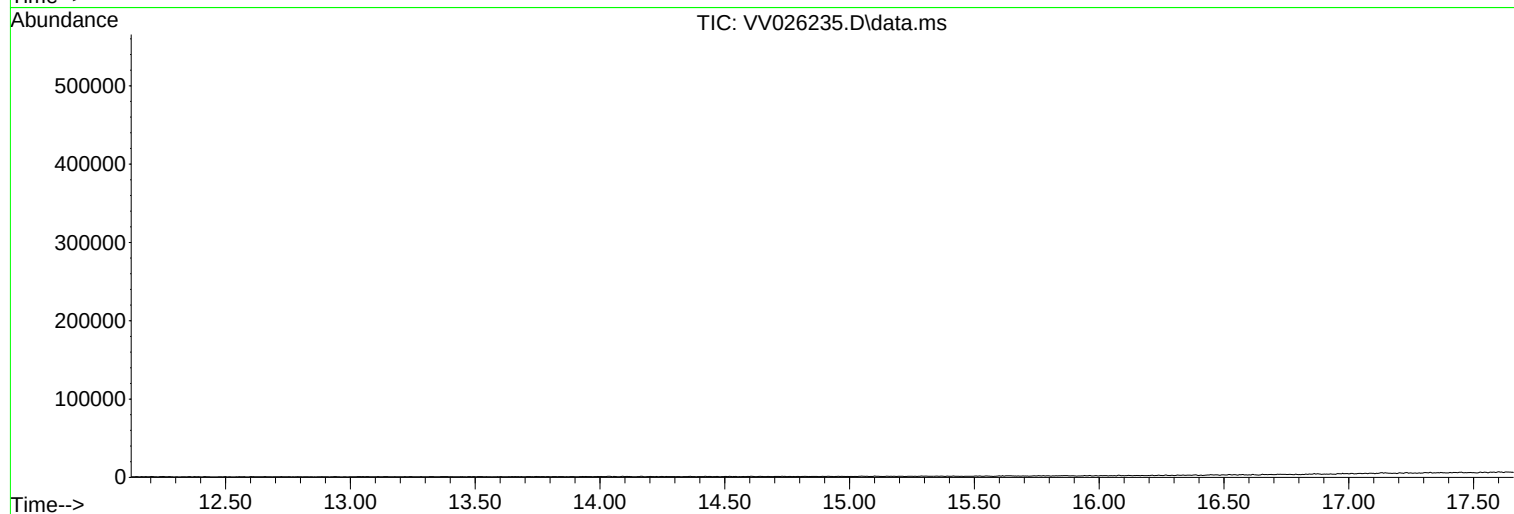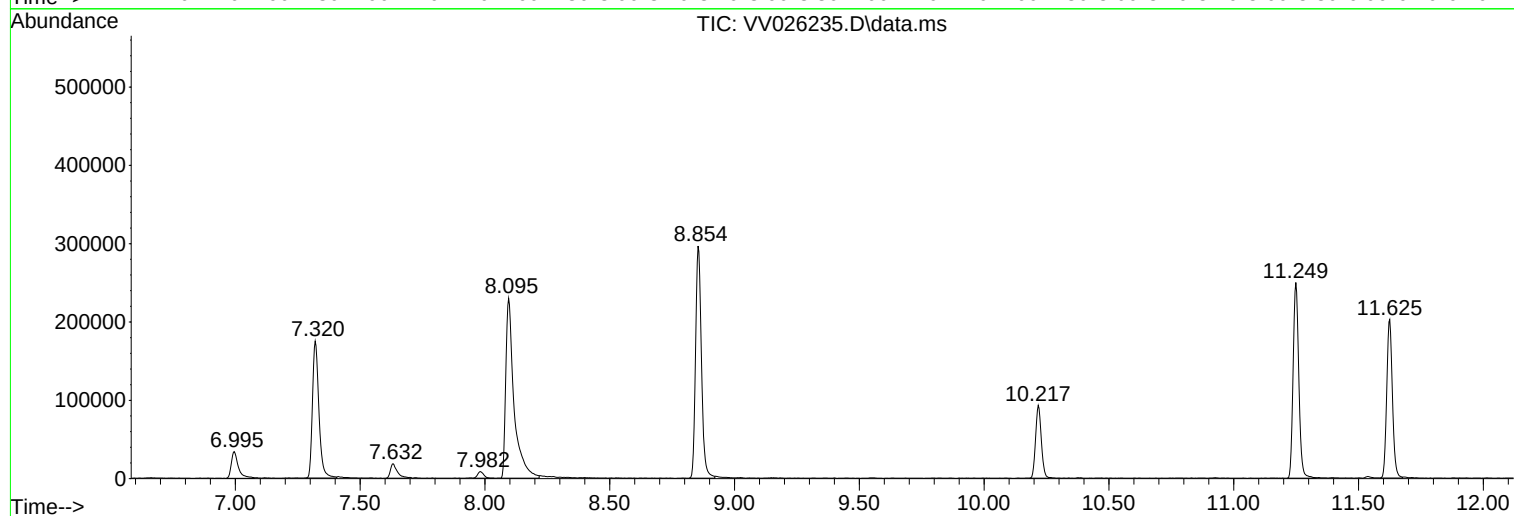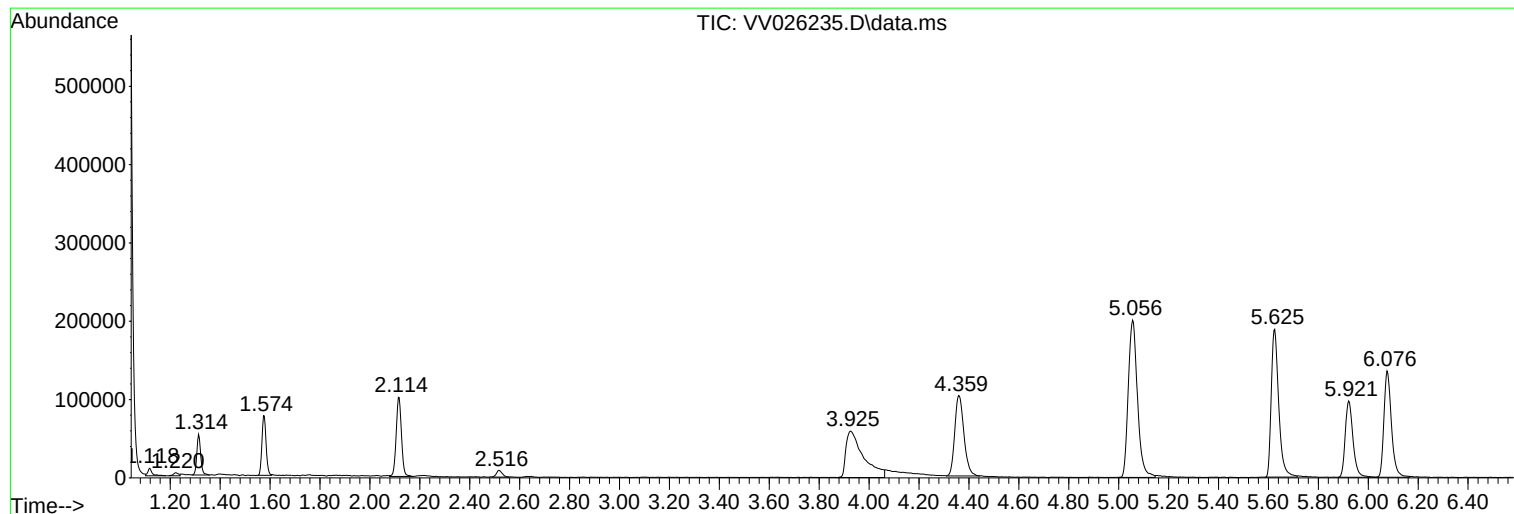

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026235.D
Acq On : 14 Jun 2022 14:30
Operator : SY/MD
Sample : N3277-09 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026235.D
Acq On : 14 Jun 2022 14:30
Operator : SY/MD
Sample : N3277-09 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc