

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026236.D
 Acq On : 14 Jun 2022 14:54
 Operator : SY/MD
 Sample : N3277-20 100X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BC7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026236.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	19	24	30	rVB	7670	6894	1.29%	0.140%
2	1.314	77	85	101	rVB	51202	55977	10.51%	1.134%
3	1.574	158	166	178	rBV	77305	88878	16.69%	1.801%
4	1.757	216	223	233	rBV	16161	20071	3.77%	0.407%
5	2.114	323	334	354	rVB	105449	153729	28.87%	3.114%
6	2.516	450	459	469	rBV2	7583	13198	2.48%	0.267%
7	3.921	877	896	929	rBV2	59124	263912	49.56%	5.347%
8	4.355	1015	1031	1062	rVB	106232	269553	50.62%	5.461%
9	5.053	1233	1248	1279	rBV3	201148	511802	96.11%	10.369%
10	5.622	1413	1425	1449	rBV	192696	396551	74.47%	8.034%
11	5.918	1502	1517	1548	rBV3	171888	352261	66.15%	7.137%
12	6.072	1553	1565	1593	rBV	135925	281256	52.82%	5.698%
13	6.992	1839	1851	1866	rBV	32685	63712	11.96%	1.291%
14	7.320	1940	1953	1974	rBV	175671	313784	58.93%	6.357%
15	7.629	2040	2049	2077	rBV2	18896	36479	6.85%	0.739%
16	7.976	2146	2157	2178	rVB	138656	235921	44.30%	4.780%
17	8.092	2181	2193	2225	rBV2	228493	532502	100.00%	10.788%
18	8.854	2419	2430	2461	rBV	296614	490285	92.07%	9.933%
19	10.217	2843	2854	2872	rBV	94698	151372	28.43%	3.067%
20	11.249	3164	3175	3196	rBV	248255	384789	72.26%	7.796%
21	11.622	3280	3291	3313	rBV	196652	313109	58.80%	6.343%




Sum of corrected areas: 4936035

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026236.D
Acq On : 14 Jun 2022 14:54
Operator : SY/MD
Sample : N3277-20 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

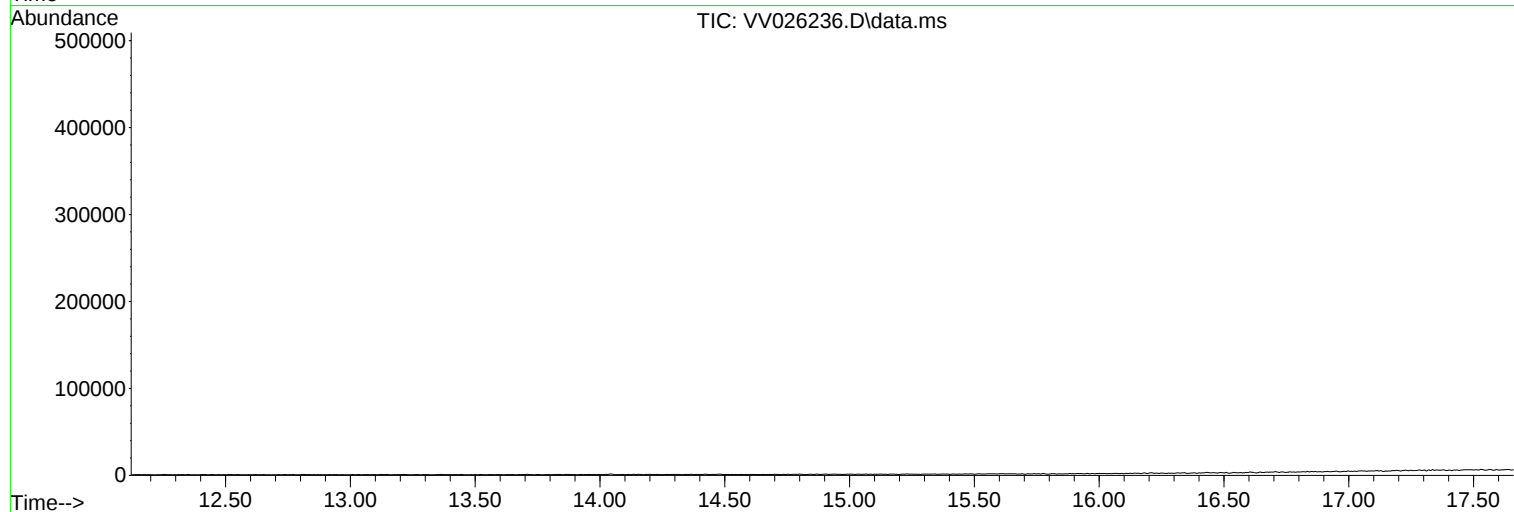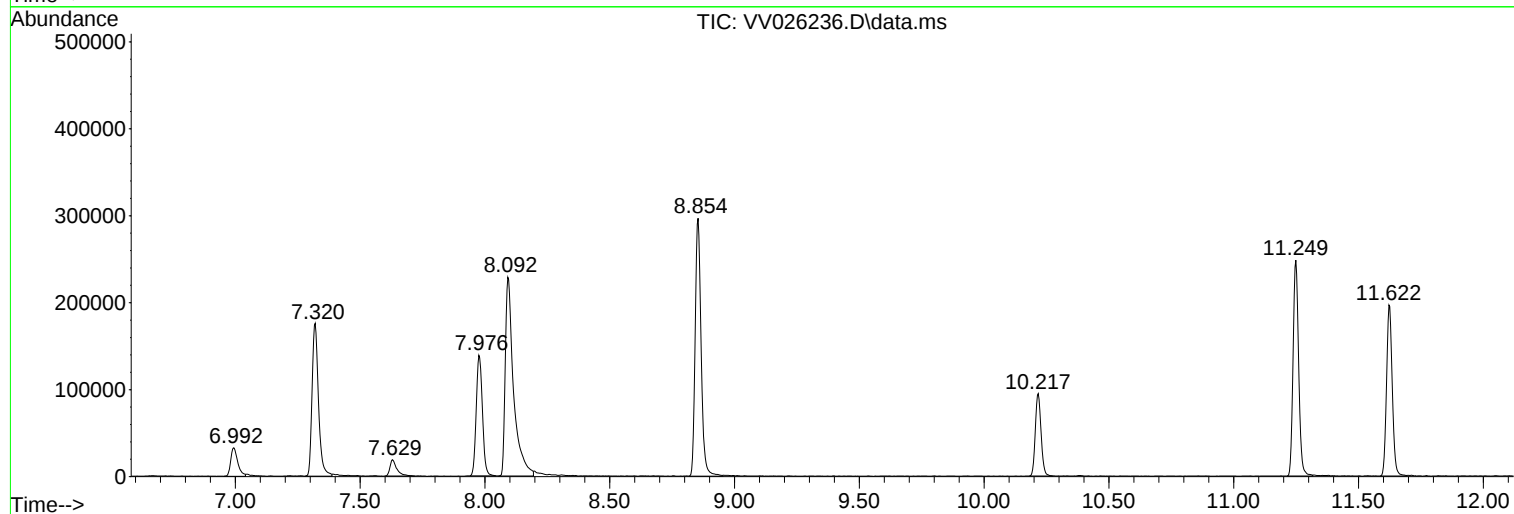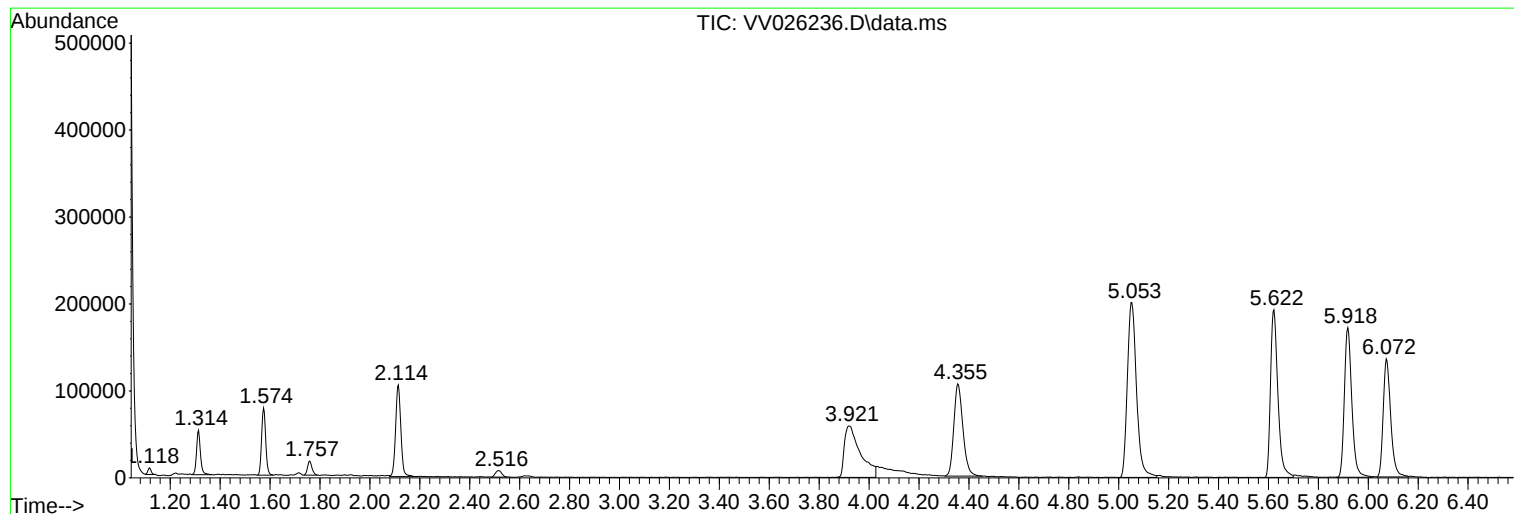

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026236.D
Acq On : 14 Jun 2022 14:54
Operator : SY/MD
Sample : N3277-20 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026236.D
Acq On : 14 Jun 2022 14:54
Operator : SY/MD
Sample : N3277-20 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
