

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026239.D
 Acq On : 14 Jun 2022 16:06
 Operator : SY/MD
 Sample : N3277-14 2000X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BB3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026239.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.314	78	85	104	rBV	121281	132468	11.56%	2.127%
2	1.574	158	166	176	rBV	109166	122848	10.72%	1.972%
3	1.761	216	224	233	rBV2	10917	14733	1.29%	0.237%
4	2.114	322	334	351	rVB	203541	294625	25.72%	4.730%
5	2.516	450	459	471	rVB2	8653	14199	1.24%	0.228%
6	3.918	879	895	923	rBV3	67555	263169	22.98%	4.225%
7	4.355	1015	1031	1059	rVB2	122332	312409	27.27%	5.015%
8	5.053	1231	1248	1290	rBV2	271678	674228	58.86%	10.824%
9	5.622	1413	1425	1444	rBV	166600	336868	29.41%	5.408%
10	5.915	1500	1516	1547	rBV	577906	1145444	100.00%	18.388%
11	6.072	1553	1565	1591	rVB	159072	325999	28.46%	5.233%
12	6.992	1839	1851	1868	rBV2	52982	102573	8.95%	1.647%
13	7.317	1940	1952	1971	rBV	289951	510717	44.59%	8.199%
14	7.629	2039	2049	2069	rBV2	29714	56093	4.90%	0.900%
15	7.979	2147	2158	2179	rVB	69483	119599	10.44%	1.920%
16	8.092	2183	2193	2236	rBV2	208444	474185	41.40%	7.612%
17	8.416	2284	2294	2309	rBV	29079	51128	4.46%	0.821%
18	8.854	2419	2430	2448	rBV	245763	411735	35.95%	6.610%
19	10.217	2843	2854	2870	rBV	94226	149673	13.07%	2.403%
20	11.249	3163	3175	3193	rBV	216950	332436	29.02%	5.337%
21	11.622	3277	3291	3308	rBV	241919	384161	33.54%	6.167%




Sum of corrected areas: 6229290

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026239.D
Acq On : 14 Jun 2022 16:06
Operator : SY/MD
Sample : N3277-14 2000X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

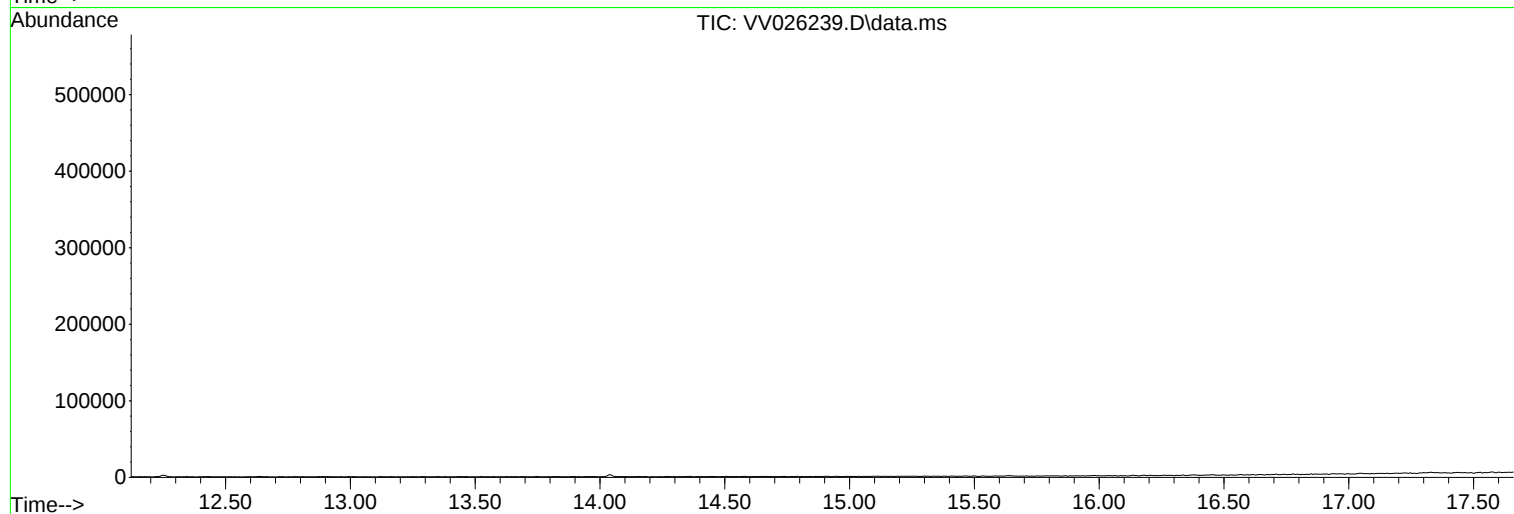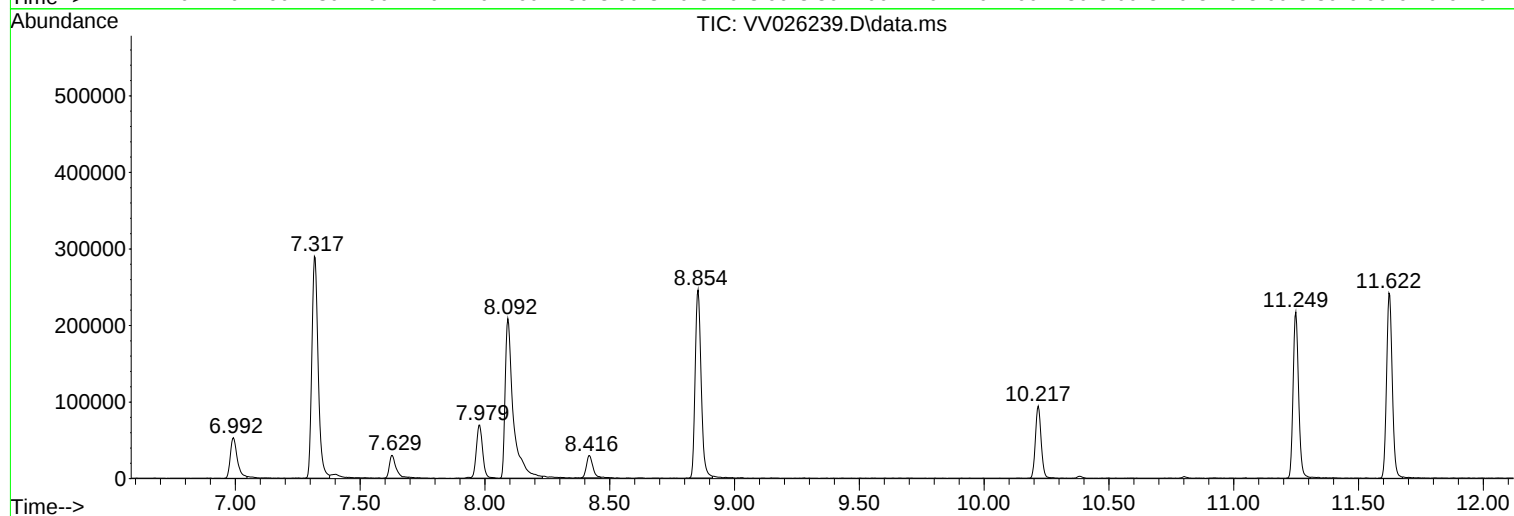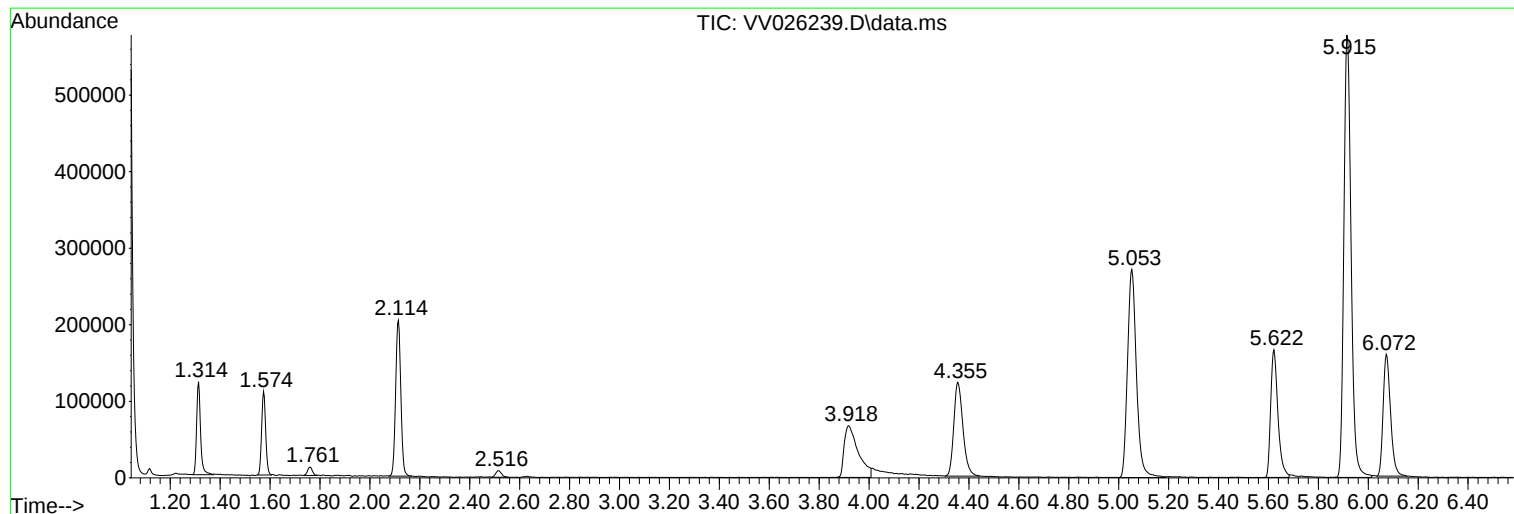

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026239.D
Acq On : 14 Jun 2022 16:06
Operator : SY/MD
Sample : N3277-14 2000X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026239.D
Acq On : 14 Jun 2022 16:06
Operator : SY/MD
Sample : N3277-14 2000X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc