

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026240.D
 Acq On : 14 Jun 2022 16:30
 Operator : SY/MD
 Sample : N3277-18 1000X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BC5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026240.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	19	24	38	rVB2	9386	10726	1.06%	0.173%
2	1.314	75	85	102	rBV	123572	137203	13.57%	2.219%
3	1.574	159	166	179	rBV	109569	125889	12.45%	2.036%
4	2.114	321	334	353	rVB	214291	308047	30.46%	4.981%
5	2.513	450	458	471	rVB2	8750	14921	1.48%	0.241%
6	3.918	879	895	926	rBV3	63193	261847	25.89%	4.234%
7	4.355	1014	1031	1062	rVB	124295	321222	31.76%	5.194%
8	5.053	1231	1248	1281	rBV2	275778	686621	67.89%	11.103%
9	5.622	1412	1425	1449	rBV	176904	362649	35.86%	5.864%
10	5.915	1502	1516	1542	rBV	510175	1011419	100.00%	16.355%
11	6.072	1552	1565	1591	rBV	161463	330020	32.63%	5.337%
12	6.992	1837	1851	1873	rBV	56332	107171	10.60%	1.733%
13	7.317	1941	1952	1972	rBV	295003	525401	51.95%	8.496%
14	7.629	2040	2049	2072	rBV2	31117	58853	5.82%	0.952%
15	7.979	2149	2158	2173	rVB2	27563	46464	4.59%	0.751%
16	8.091	2182	2193	2235	rBV	215959	477022	47.16%	7.714%
17	8.419	2285	2295	2312	rBV2	20787	37945	3.75%	0.614%
18	8.854	2419	2430	2454	rBV	276304	449185	44.41%	7.264%
19	10.217	2842	2854	2869	rBV2	96099	153483	15.18%	2.482%
20	11.249	3164	3175	3193	rBV	230833	359720	35.57%	5.817%
21	11.622	3279	3291	3311	rBV	253449	398294	39.38%	6.441%




Sum of corrected areas: 6184102

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026240.D
Acq On : 14 Jun 2022 16:30
Operator : SY/MD
Sample : N3277-18 1000X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

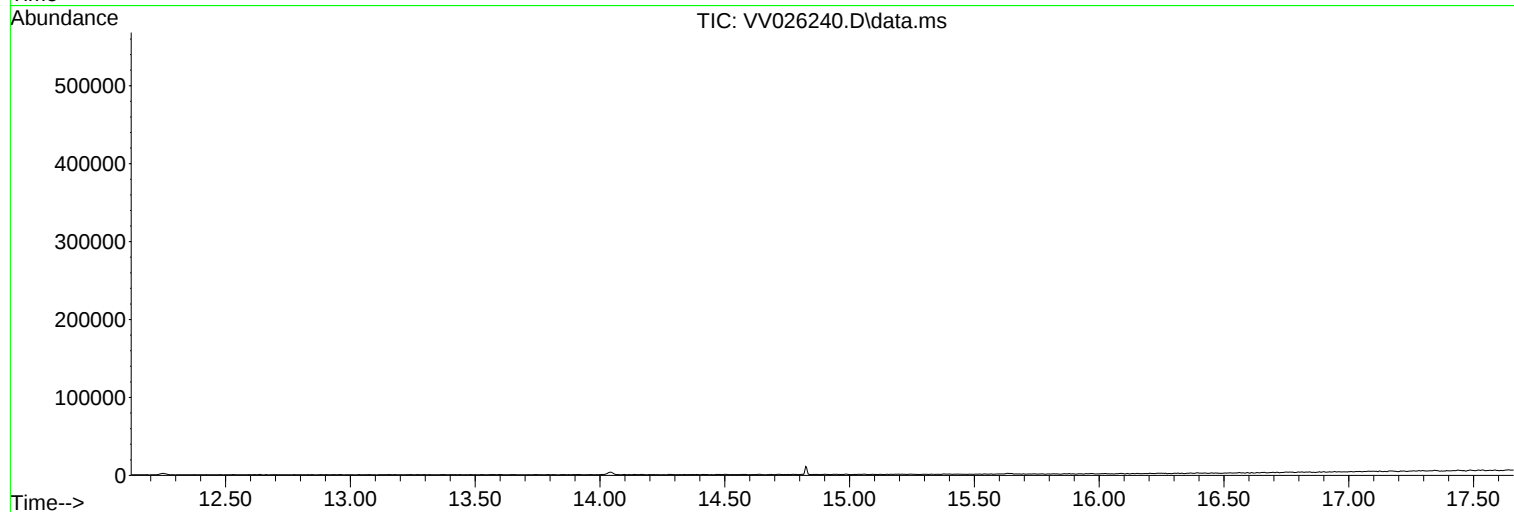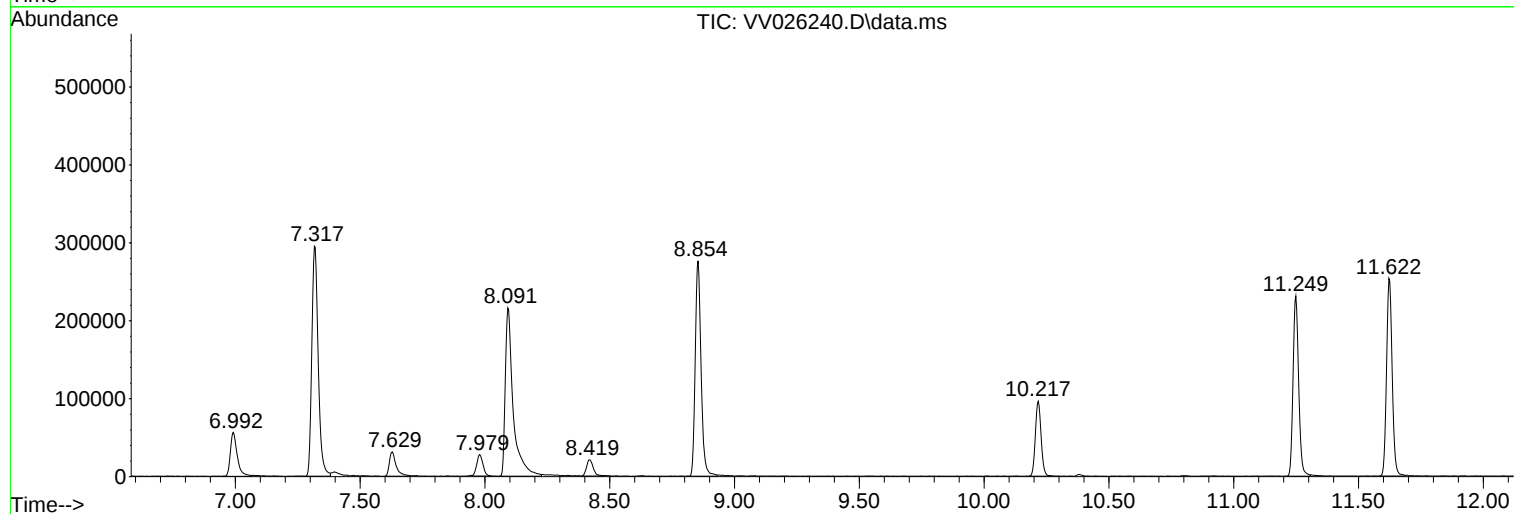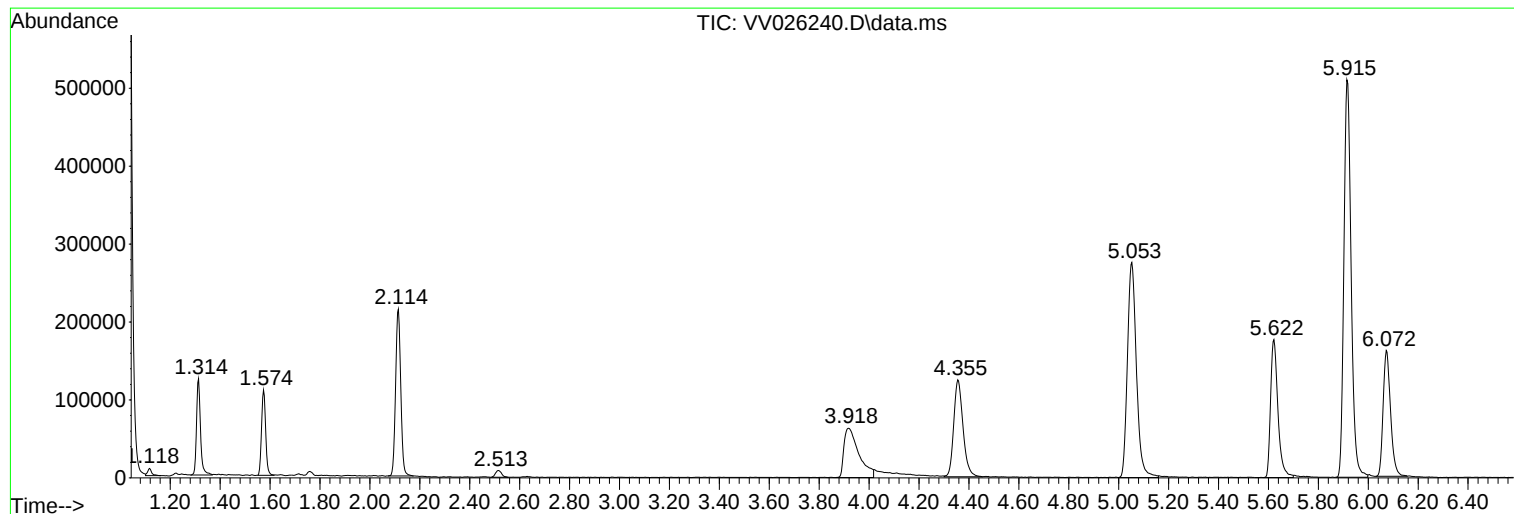

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026240.D
Acq On : 14 Jun 2022 16:30
Operator : SY/MD
Sample : N3277-18 1000X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026240.D
Acq On : 14 Jun 2022 16:30
Operator : SY/MD
Sample : N3277-18 1000X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
