

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026241.D
 Acq On : 14 Jun 2022 16:54
 Operator : SY/MD
 Sample : N3277-19 1000X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BC6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026241.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.314	76	85	102	rBV	120648	132426	13.61%	2.161%
2	1.574	157	166	181	rBV	109321	124596	12.81%	2.033%
3	2.114	323	334	353	rVB	207066	300355	30.87%	4.902%
4	2.513	448	458	473	rVB2	11636	21597	2.22%	0.352%
5	3.924	879	897	931	rBV3	67423	315025	32.38%	5.141%
6	4.355	1014	1031	1066	rVB	123080	315577	32.44%	5.150%
7	5.053	1232	1248	1280	rBV2	272974	672491	69.13%	10.975%
8	5.622	1413	1425	1449	rBV	174808	360916	37.10%	5.890%
9	5.915	1503	1516	1550	rBV	484520	972849	100.00%	15.877%
10	6.072	1553	1565	1592	rVB	157111	323891	33.29%	5.286%
11	6.992	1841	1851	1872	rBV	53579	102473	10.53%	1.672%
12	7.317	1940	1952	1974	rBV	292480	516612	53.10%	8.431%
13	7.628	2037	2049	2070	rBV	31894	58675	6.03%	0.958%
14	7.979	2149	2158	2174	rVB3	26963	46510	4.78%	0.759%
15	8.091	2183	2193	2228	rBV2	211301	461468	47.43%	7.531%
16	8.419	2285	2295	2315	rBV2	31716	55937	5.75%	0.913%
17	8.854	2418	2430	2453	rBV	265873	443321	45.57%	7.235%
18	10.217	2843	2854	2871	rBV	94038	149800	15.40%	2.445%
19	11.249	3164	3175	3199	rBV	229235	359516	36.95%	5.867%
20	11.625	3279	3292	3313	rBV	244149	393265	40.42%	6.418%




Sum of corrected areas: 6127300

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026241.D
Acq On : 14 Jun 2022 16:54
Operator : SY/MD
Sample : N3277-19 1000X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

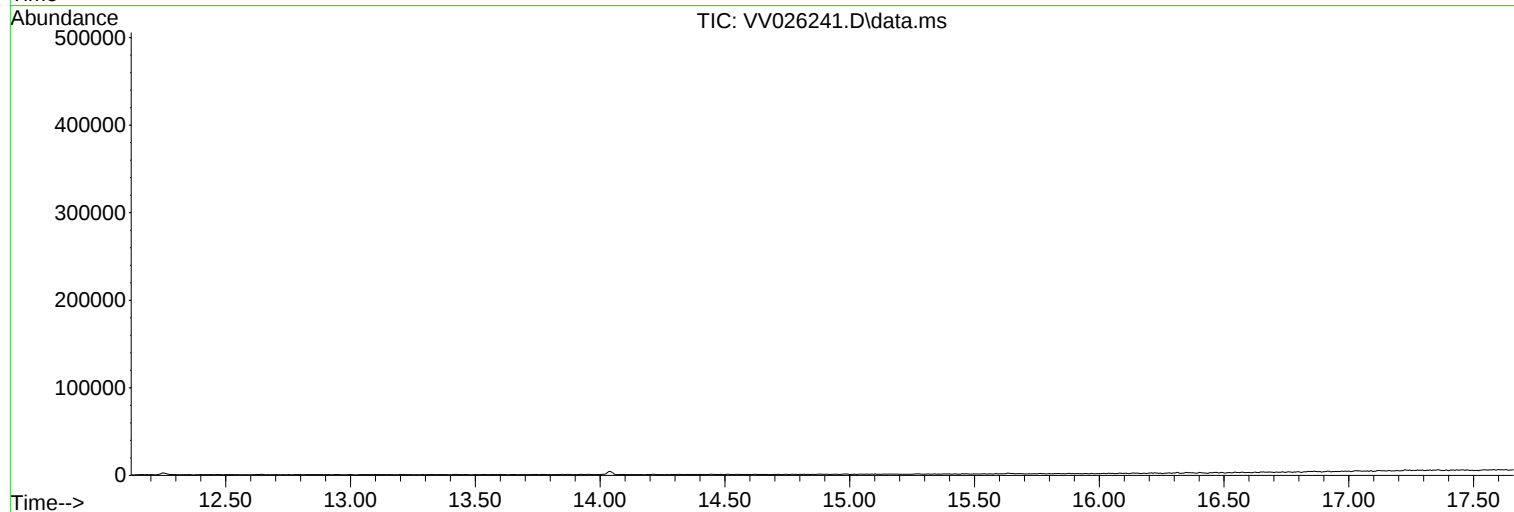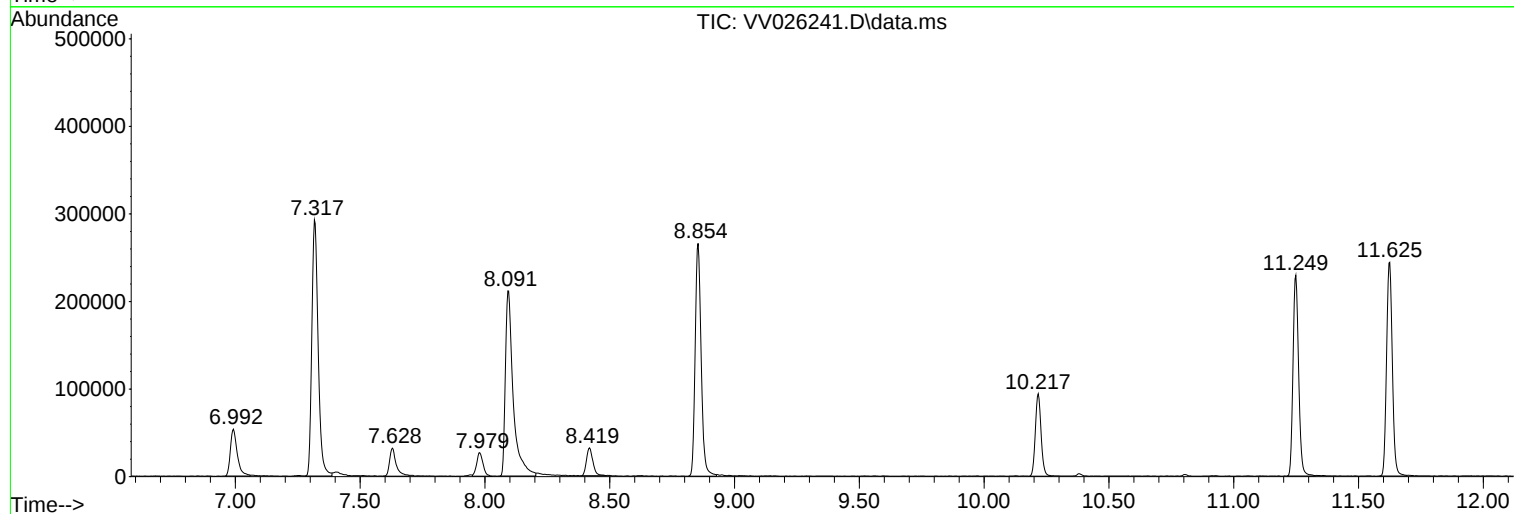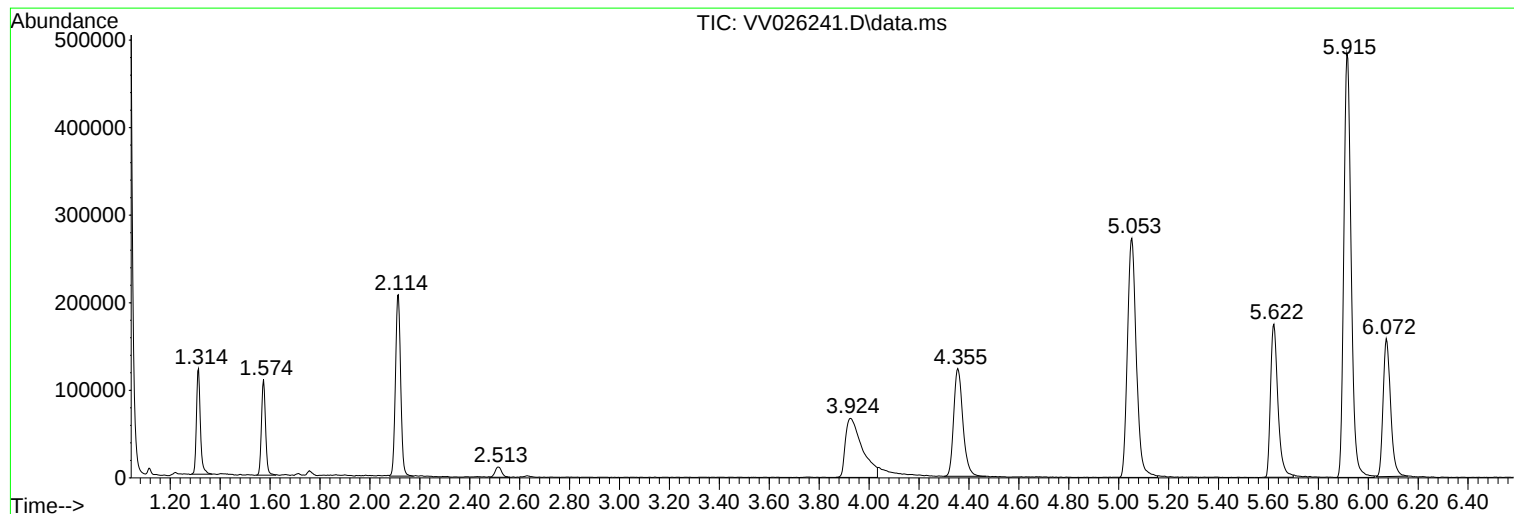

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026241.D
Acq On : 14 Jun 2022 16:54
Operator : SY/MD
Sample : N3277-19 1000X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026241.D
Acq On : 14 Jun 2022 16:54
Operator : SY/MD
Sample : N3277-19 1000X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
