

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026245.D
 Acq On : 14 Jun 2022 19:17
 Operator : SY/MD
 Sample : N3272-15DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B59DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026245.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	19	24	39	rVB4	8980	10855	1.33%	0.165%
2	1.314	76	85	100	rBV	140815	151578	18.51%	2.305%
3	1.574	158	166	183	rBV	127778	145804	17.80%	2.217%
4	1.761	215	224	235	rVB	25504	33471	4.09%	0.509%
5	2.114	322	334	350	rBV	239472	345855	42.23%	5.259%
6	2.513	448	458	473	rVB	26671	43530	5.32%	0.662%
7	3.915	882	894	931	rBV2	55834	238767	29.16%	3.630%
8	4.355	1015	1031	1055	rBV	148332	373045	45.55%	5.672%
9	5.053	1229	1248	1288	rBV2	328661	818915	100.00%	12.451%
10	5.622	1412	1425	1452	rBV	188350	388247	47.41%	5.903%
11	5.918	1503	1517	1546	rBV2	222377	457098	55.82%	6.950%
12	6.072	1552	1565	1592	rBV	187318	386884	47.24%	5.882%
13	6.989	1834	1850	1871	rBV	74704	143670	17.54%	2.184%
14	7.317	1941	1952	1973	rBV	359695	639689	78.11%	9.726%
15	7.625	2039	2048	2078	rBV	42822	81057	9.90%	1.232%
16	7.976	2135	2157	2174	rBV	101471	181932	22.22%	2.766%
17	8.092	2183	2193	2233	rBV2	261572	585894	71.55%	8.908%
18	8.854	2418	2430	2456	rBV	284376	476389	58.17%	7.243%
19	10.217	2840	2854	2873	rBV	116269	183766	22.44%	2.794%
20	10.384	2894	2906	2915	rBV2	6778	11284	1.38%	0.172%
21	11.249	3164	3175	3197	rBV	255305	391730	47.84%	5.956%
22	11.622	3280	3291	3317	rBV	311354	487565	59.54%	7.413%




Sum of corrected areas: 6577025

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026245.D
Acq On : 14 Jun 2022 19:17
Operator : SY/MD
Sample : N3272-15DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B59DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

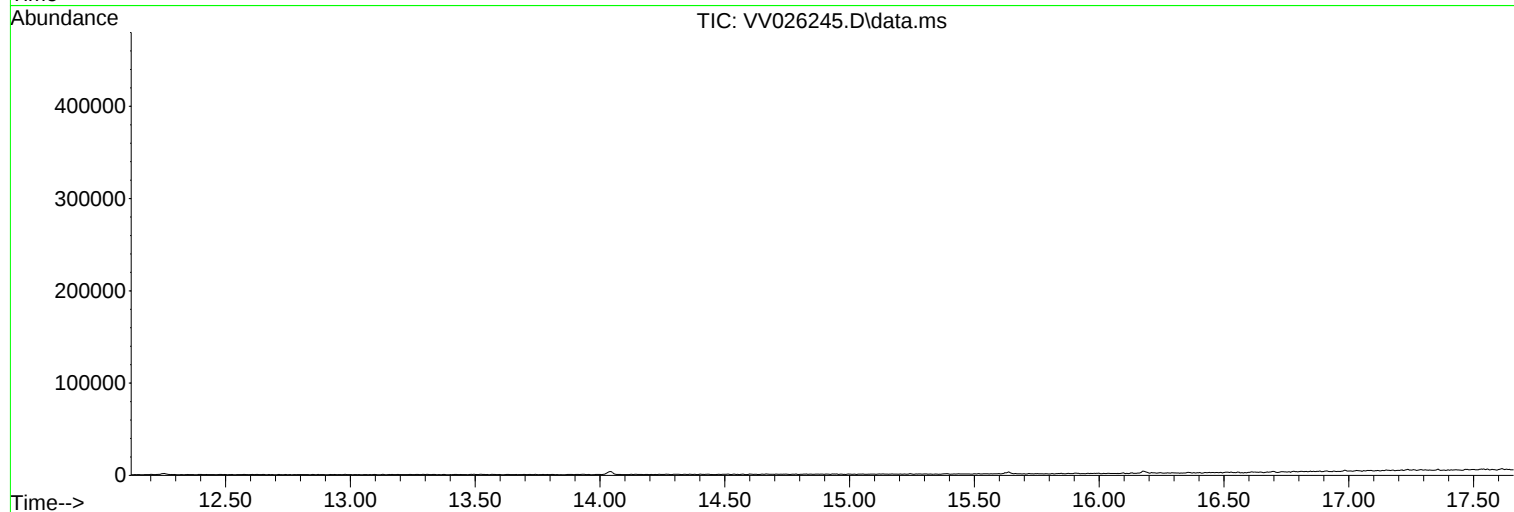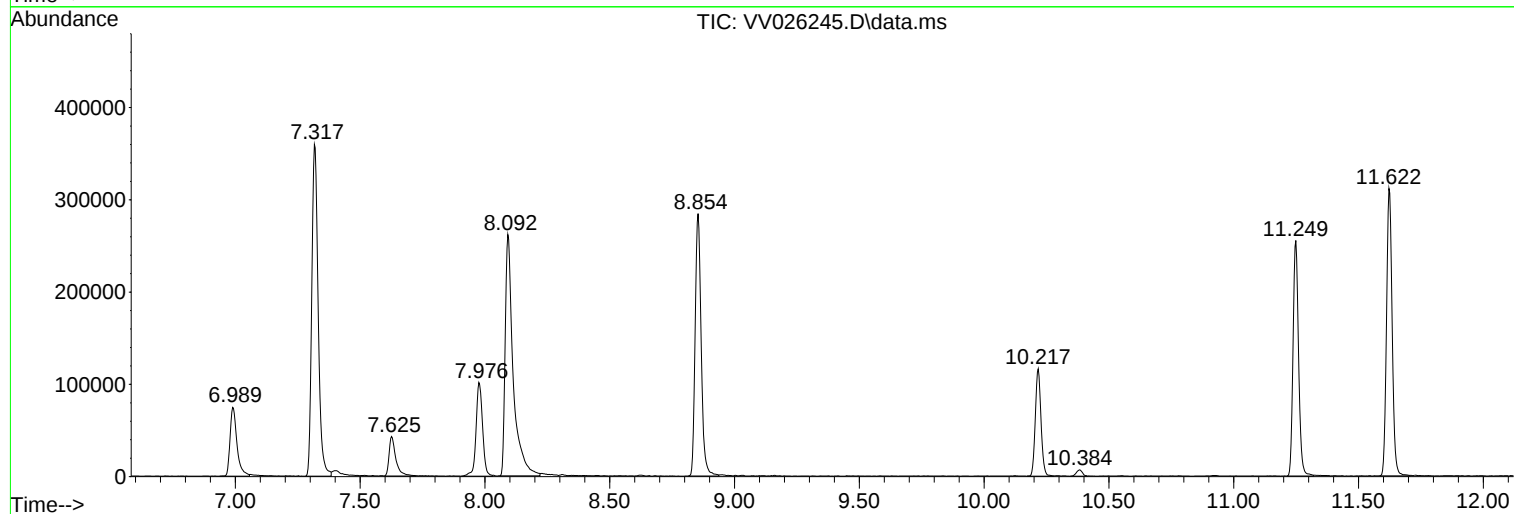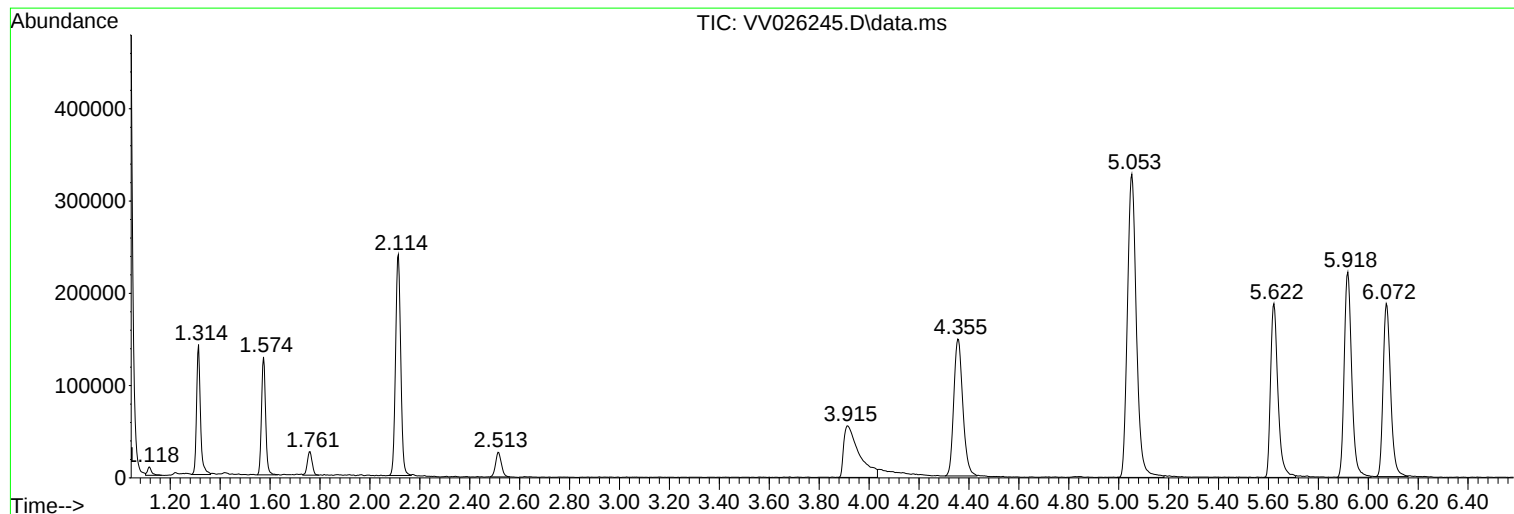

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026245.D
Acq On : 14 Jun 2022 19:17
Operator : SY/MD
Sample : N3272-15DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B59DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026245.D
Acq On : 14 Jun 2022 19:17
Operator : SY/MD
Sample : N3272-15DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B59DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc