

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026246.D
 Acq On : 14 Jun 2022 19:41
 Operator : SY/MD
 Sample : N3272-21
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026246.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.117	19	24	34	rVB2	8678	9471	1.20%	0.167%
2	1.314	78	85	100	rVB	134356	144275	18.27%	2.548%
3	1.574	158	166	181	rBV	124035	142228	18.01%	2.512%
4	2.114	323	334	354	rVB	239855	343802	43.53%	6.071%
5	2.516	448	459	476	rBV	12229	21497	2.72%	0.380%
6	3.918	883	895	932	rBV	48068	217565	27.54%	3.842%
7	4.355	1014	1031	1062	rBB	142029	361264	45.74%	6.380%
8	5.053	1229	1248	1281	rBV2	323009	789858	100.00%	13.948%
9	5.622	1413	1425	1458	rBV	175461	367088	46.48%	6.482%
10	5.915	1504	1516	1532	rBV4	9528	20966	2.65%	0.370%
11	6.072	1551	1565	1589	rBV	181627	377360	47.78%	6.664%
12	6.989	1840	1850	1872	rBV2	70533	136104	17.23%	2.403%
13	7.317	1940	1952	1972	rBV	348398	609786	77.20%	10.768%
14	7.625	2039	2048	2069	rBV2	40907	74822	9.47%	1.321%
15	7.943	2136	2147	2156	rBV3	4758	8685	1.10%	0.153%
16	8.091	2182	2193	2231	rBV2	261251	564989	71.53%	9.977%
17	8.853	2419	2430	2453	rBV	271641	450406	57.02%	7.954%
18	10.217	2843	2854	2867	rBV	111069	175628	22.24%	3.101%
19	10.381	2895	2905	2915	rBV3	9498	14210	1.80%	0.251%
20	11.249	3164	3175	3202	rBV	238101	369598	46.79%	6.527%
21	11.622	3280	3291	3309	rBV	291402	463235	58.65%	8.180%




Sum of corrected areas: 5662837

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026246.D
Acq On : 14 Jun 2022 19:41
Operator : SY/MD
Sample : N3272-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

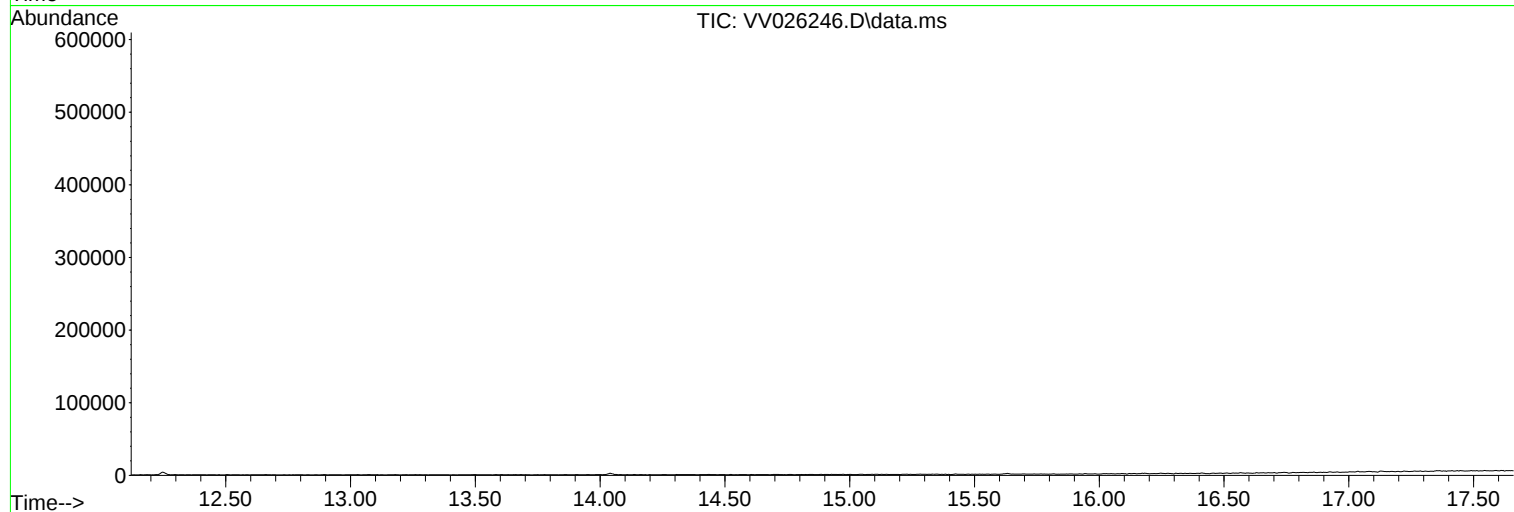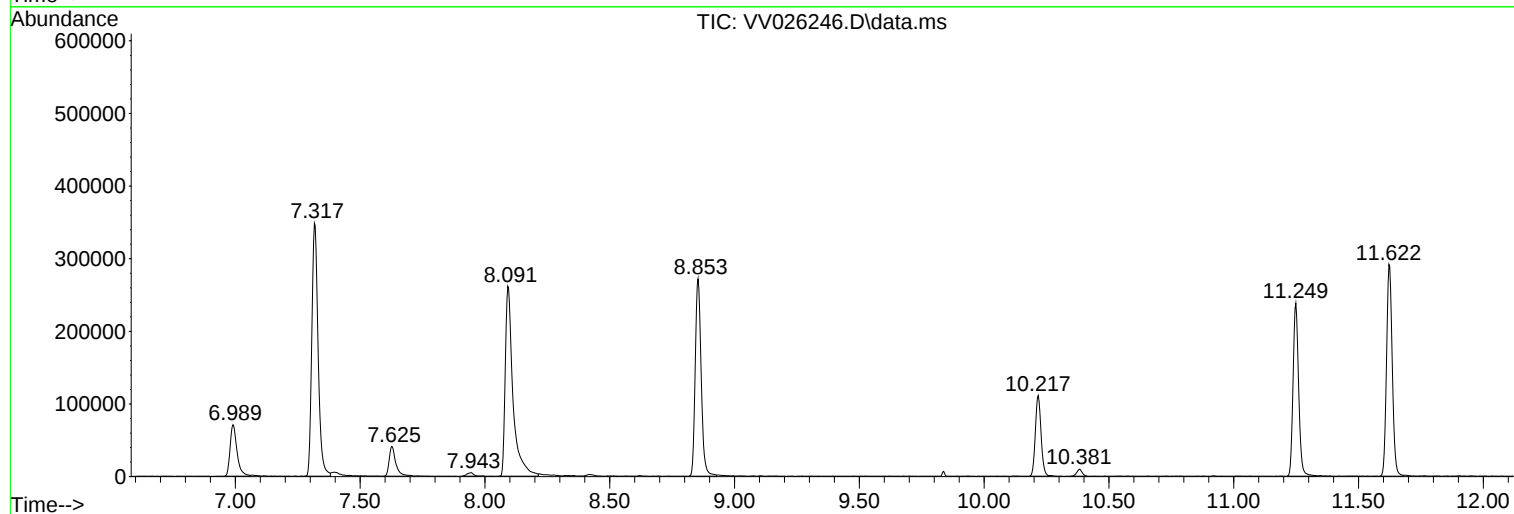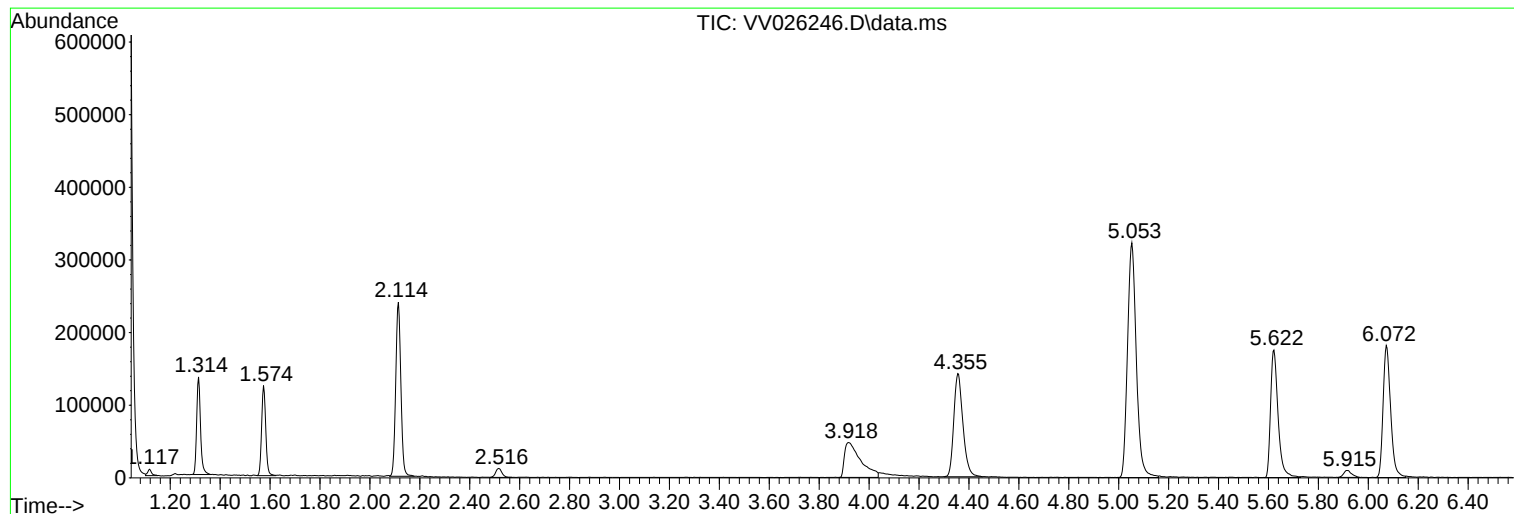

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026246.D
Acq On : 14 Jun 2022 19:41
Operator : SY/MD
Sample : N3272-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026246.D
Acq On : 14 Jun 2022 19:41
Operator : SY/MD
Sample : N3272-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc