

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026249.D
 Acq On : 14 Jun 2022 21:19
 Operator : SY/MD
 Sample : N3273-09DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B79DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026249.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.117	19	24	31	rVB3	9212	9250	1.15%	0.160%
2	1.314	78	85	109	rVB	134056	146899	18.22%	2.548%
3	1.574	158	166	182	rVB	123714	141839	17.59%	2.460%
4	2.114	323	334	353	rVB	236361	337412	41.85%	5.852%
5	2.516	450	459	470	rVB2	6939	11963	1.48%	0.207%
6	3.921	880	896	921	rBV2	60203	253363	31.43%	4.394%
7	4.355	1015	1031	1064	rVB	146026	369542	45.84%	6.409%
8	5.053	1232	1248	1279	rBV3	324067	806156	100.00%	13.981%
9	5.622	1414	1425	1450	rBV	179214	367994	45.65%	6.382%
10	5.918	1505	1517	1532	rVB7	9809	21835	2.71%	0.379%
11	6.072	1553	1565	1593	rBV	189897	389089	48.26%	6.748%
12	6.989	1840	1850	1871	rBV	72427	138727	17.21%	2.406%
13	7.317	1941	1952	1973	rBV	356305	620670	76.99%	10.764%
14	7.625	2039	2048	2065	rBV2	42674	78860	9.78%	1.368%
15	8.091	2183	2193	2228	rBV2	275364	583149	72.34%	10.113%
16	8.853	2418	2430	2455	rBV	271169	449533	55.76%	7.796%
17	10.217	2840	2854	2871	rBV	113752	183812	22.80%	3.188%
18	11.249	3164	3175	3201	rBV	240282	370970	46.02%	6.434%
19	11.622	3279	3291	3309	rBV	298848	485092	60.17%	8.413%




Sum of corrected areas: 5766155

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026249.D
Acq On : 14 Jun 2022 21:19
Operator : SY/MD
Sample : N3273-09DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B79DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

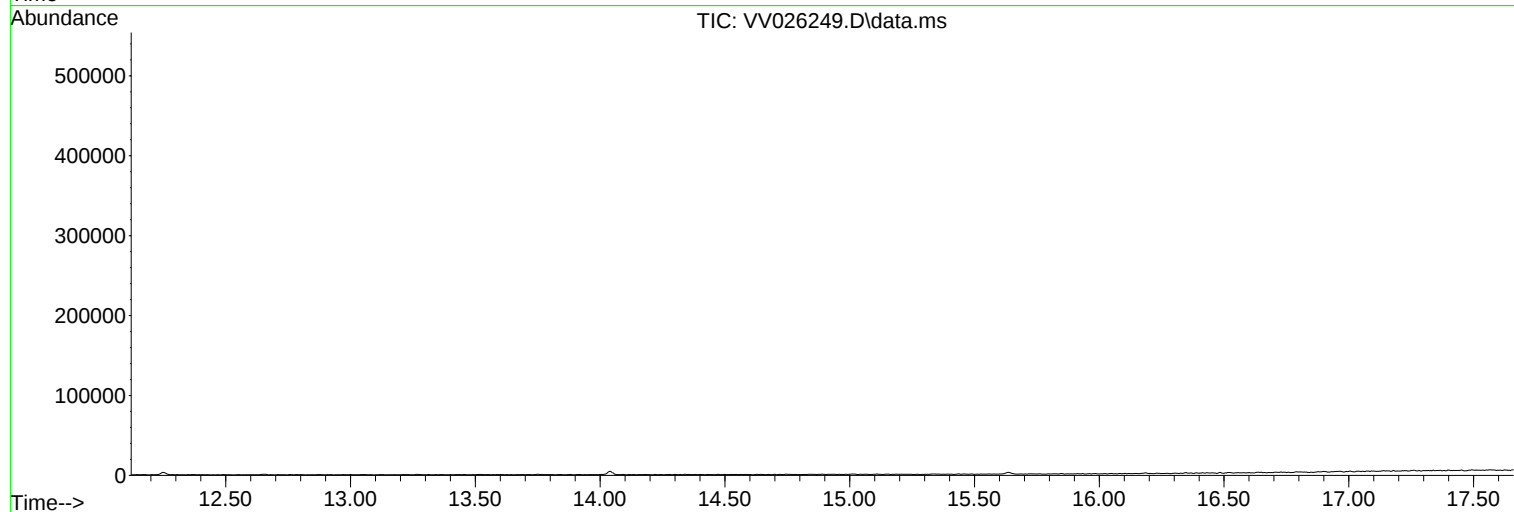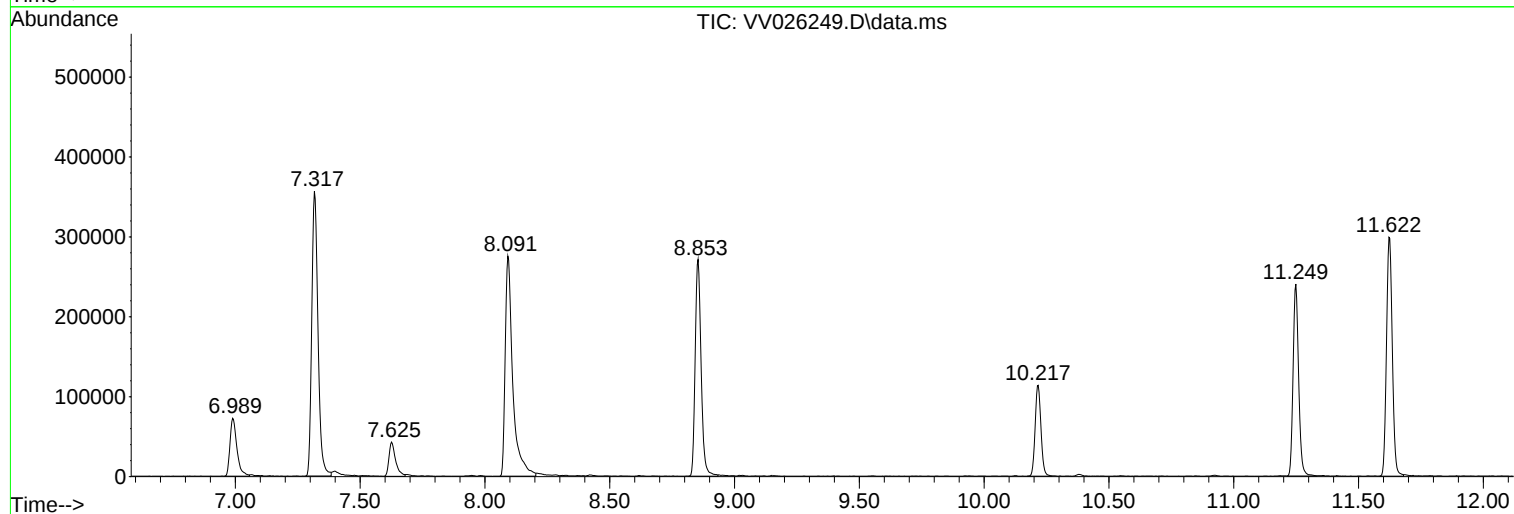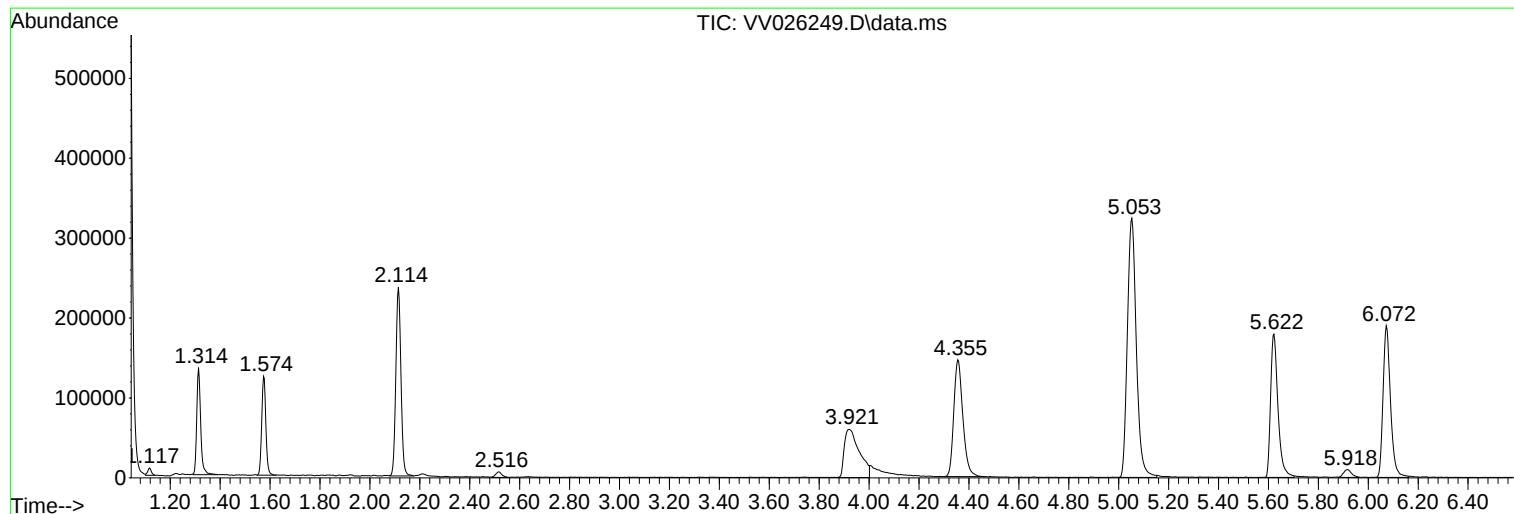

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026249.D
Acq On : 14 Jun 2022 21:19
Operator : SY/MD
Sample : N3273-09DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B79DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026249.D
Acq On : 14 Jun 2022 21:19
Operator : SY/MD
Sample : N3273-09DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B79DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
