

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026250.D
 Acq On : 14 Jun 2022 21:43
 Operator : SY/MD
 Sample : N3273-10DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B80DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026250.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	19	24	39	rVB3	8894	10502	1.38%	0.191%
2	1.314	77	85	100	rBV	126777	134998	17.75%	2.449%
3	1.574	158	166	180	rBV	118346	135599	17.82%	2.460%
4	2.114	323	334	354	rVB	222096	318716	41.90%	5.783%
5	2.516	450	459	470	rVB4	5583	9148	1.20%	0.166%
6	3.915	879	894	925	rBV2	59238	239158	31.44%	4.339%
7	4.355	1015	1031	1062	rVB	139932	351680	46.23%	6.381%
8	5.053	1232	1248	1277	rBV2	305718	760744	100.00%	13.803%
9	5.622	1413	1425	1451	rBV	179822	369887	48.62%	6.711%
10	5.915	1506	1516	1539	rVB5	9121	20458	2.69%	0.371%
11	6.072	1552	1565	1589	rBV	175328	364875	47.96%	6.620%
12	6.989	1839	1850	1875	rBV	68718	131453	17.28%	2.385%
13	7.317	1940	1952	1972	rBV	332462	589801	77.53%	10.701%
14	7.625	2038	2048	2072	rBV	40122	75729	9.95%	1.374%
15	8.092	2183	2193	2241	rBV2	242072	548770	72.14%	9.957%
16	8.854	2417	2430	2456	rBV	276092	453576	59.62%	8.230%
17	10.217	2843	2854	2870	rBV	107014	172173	22.63%	3.124%
18	11.249	3164	3175	3198	rBV	235771	366776	48.21%	6.655%
19	11.622	3280	3291	3309	rBV	295080	457423	60.13%	8.299%




Sum of corrected areas: 5511466

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026250.D
Acq On : 14 Jun 2022 21:43
Operator : SY/MD
Sample : N3273-10DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B80DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

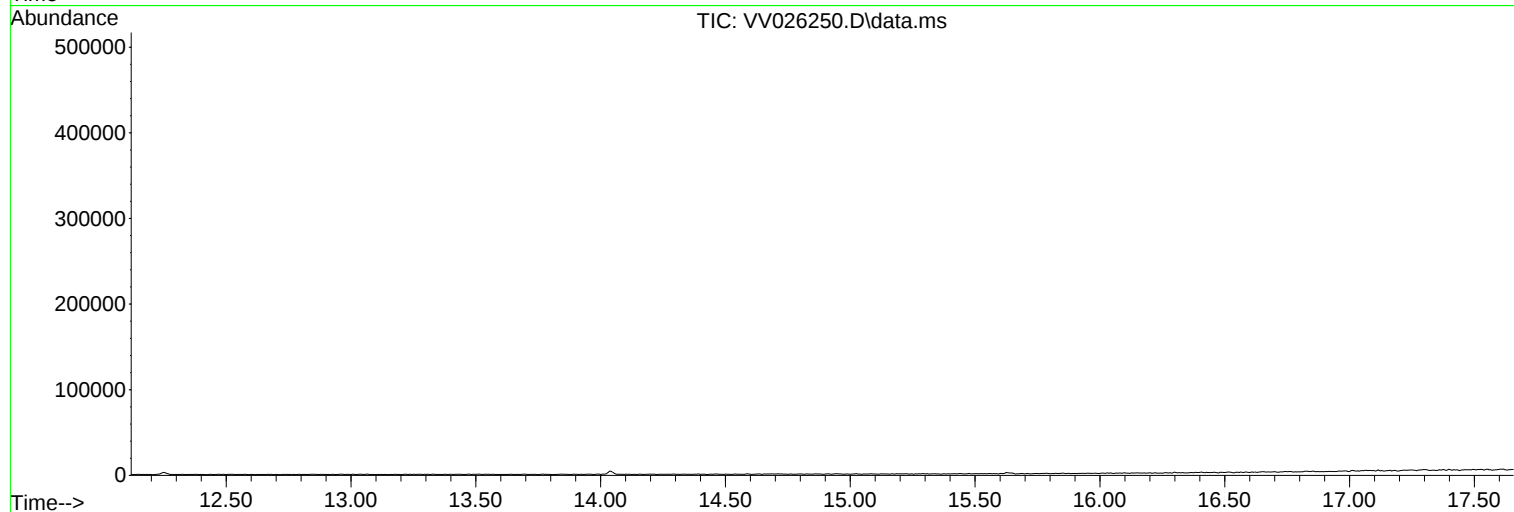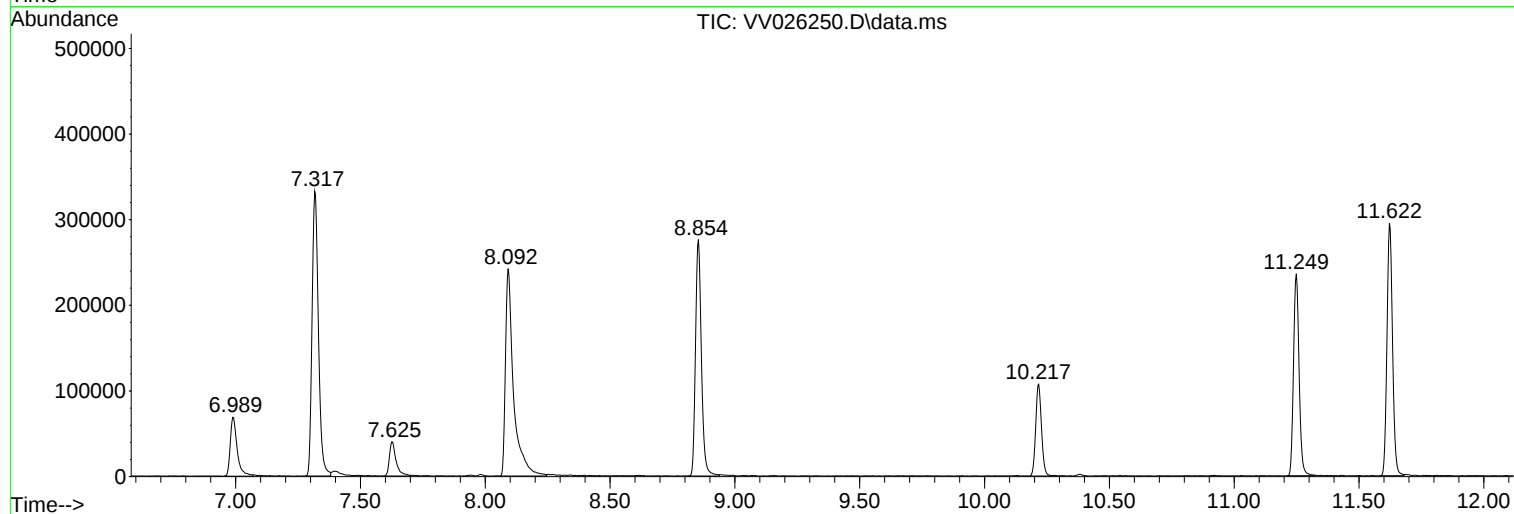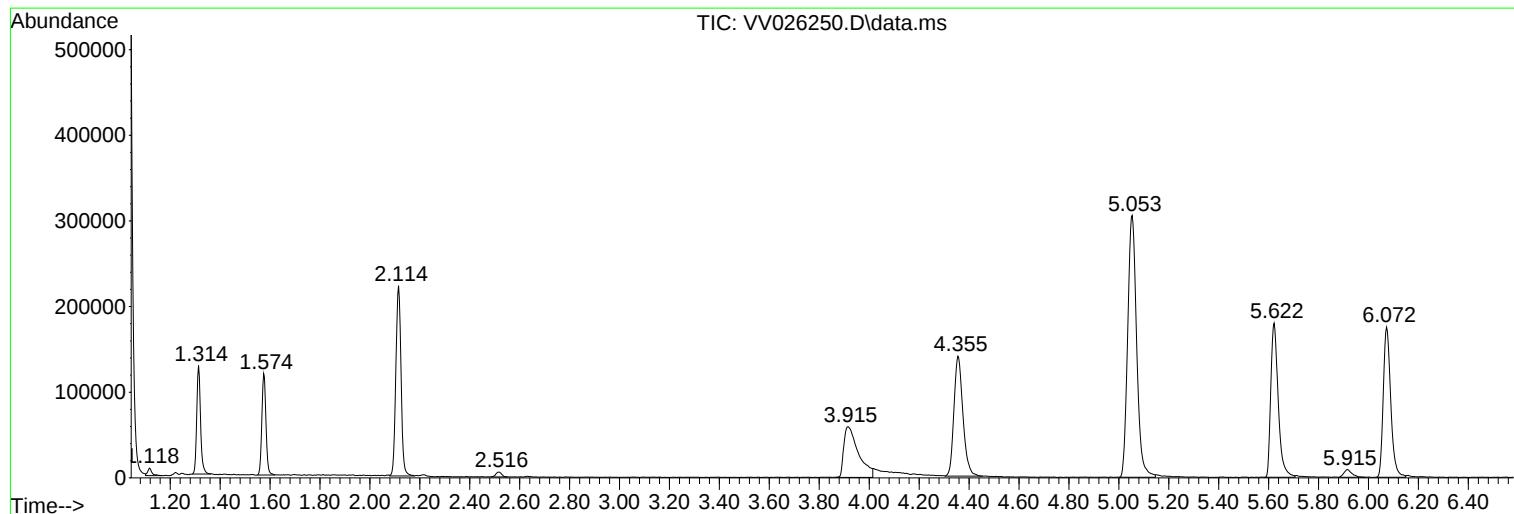

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026250.D
Acq On : 14 Jun 2022 21:43
Operator : SY/MD
Sample : N3273-10DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B80DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026250.D
Acq On : 14 Jun 2022 21:43
Operator : SY/MD
Sample : N3273-10DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B80DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
