

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026251.D
 Acq On : 14 Jun 2022 22:13
 Operator : SY/MD
 Sample : N3275-03 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026251.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	19	24	33	rVB	8702	9353	1.20%	0.165%
2	1.310	77	84	106	rVB	124884	140854	18.15%	2.488%
3	1.574	158	166	181	rVB	116888	135007	17.39%	2.385%
4	2.111	322	333	351	rVB	232286	329458	42.44%	5.820%
5	2.513	450	458	470	rBV2	6023	10069	1.30%	0.178%
6	3.908	880	892	927	rBV2	53068	220537	28.41%	3.896%
7	4.352	1014	1030	1058	rVB	142864	359865	46.36%	6.357%
8	5.050	1231	1247	1279	rBV2	309863	776260	100.00%	13.713%
9	5.619	1412	1424	1452	rBV	190794	396855	51.12%	7.011%
10	5.912	1504	1515	1533	rVB9	10358	22927	2.95%	0.405%
11	6.069	1549	1564	1595	rBV2	181981	376139	48.46%	6.645%
12	6.985	1840	1849	1866	rBV	70045	131472	16.94%	2.323%
13	7.317	1939	1952	1973	rBV	345149	603493	77.74%	10.661%
14	7.625	2039	2048	2065	rBV2	40098	74397	9.58%	1.314%
15	8.092	2177	2193	2227	rBV2	234956	555259	71.53%	9.809%
16	8.850	2419	2429	2447	rBV	297859	482124	62.11%	8.517%
17	10.214	2838	2853	2872	rBV	105573	170496	21.96%	3.012%
18	11.249	3161	3175	3195	rBV	255980	396967	51.14%	7.013%
19	11.622	3277	3291	3318	rBV	289585	469116	60.43%	8.287%




Sum of corrected areas: 5660648

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026251.D
Acq On : 14 Jun 2022 22:13
Operator : SY/MD
Sample : N3275-03 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

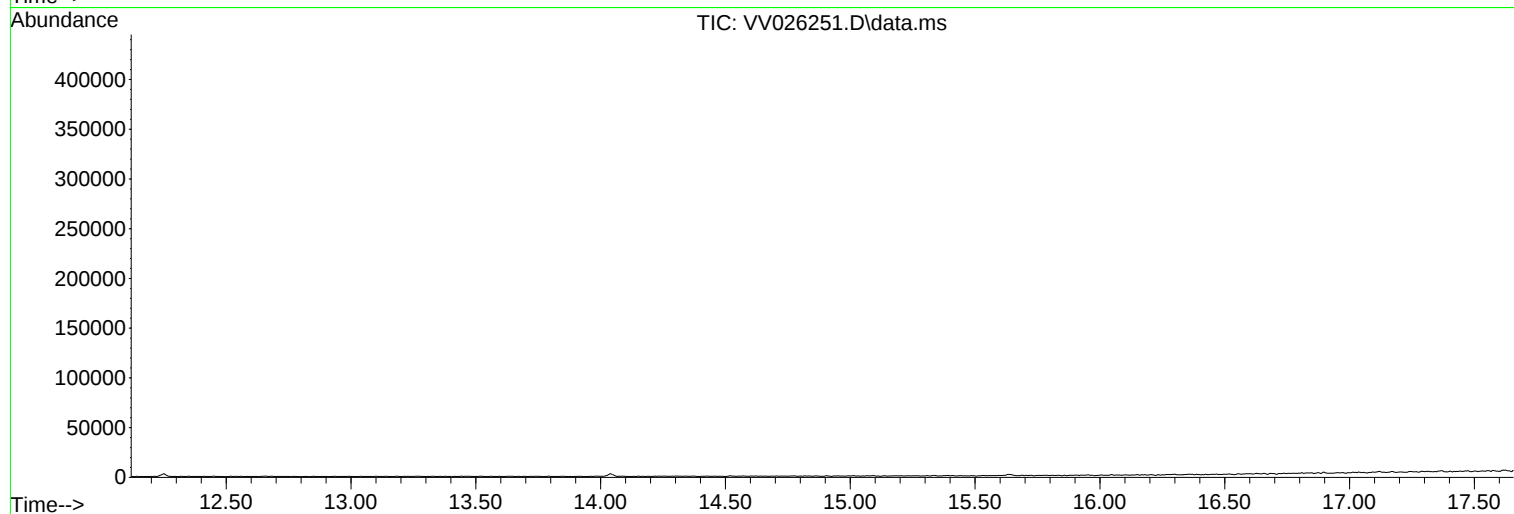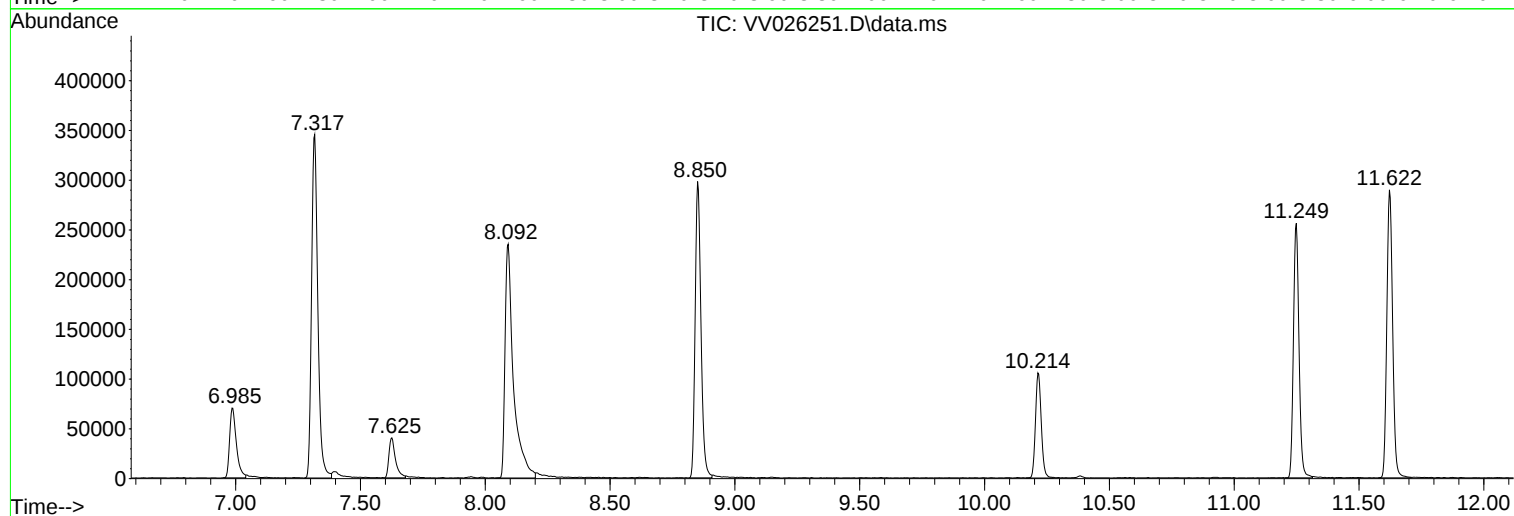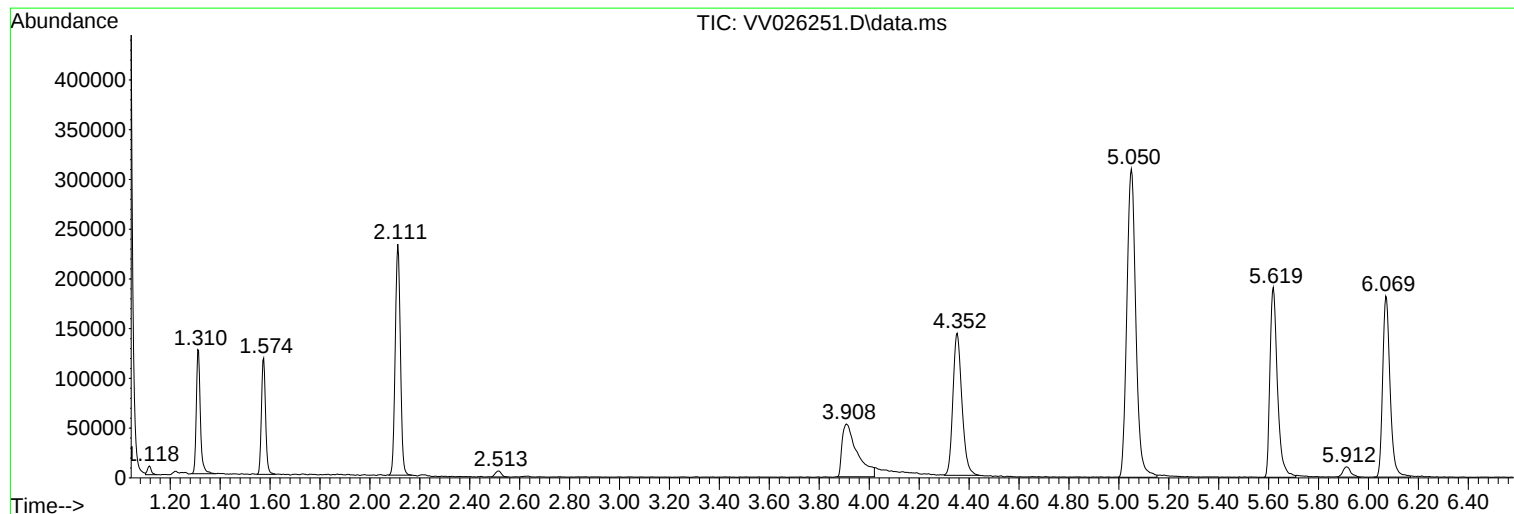

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026251.D
Acq On : 14 Jun 2022 22:13
Operator : SY/MD
Sample : N3275-03 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026251.D
Acq On : 14 Jun 2022 22:13
Operator : SY/MD
Sample : N3275-03 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc