

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026252.D
 Acq On : 14 Jun 2022 22:36
 Operator : SY/MD
 Sample : N3275-04 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026252.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	19	24	39	rVB3	9085	10416	1.36%	0.185%
2	1.314	77	85	99	rBV	122629	133776	17.48%	2.373%
3	1.574	158	166	180	rBV	113443	131317	17.16%	2.329%
4	2.114	323	334	351	rBV	219974	313043	40.91%	5.553%
5	2.516	448	459	468	rBV2	5252	8462	1.11%	0.150%
6	3.915	882	894	932	rBV3	65435	278253	36.36%	4.935%
7	4.355	1012	1031	1063	rVB	138848	355171	46.42%	6.300%
8	5.053	1232	1248	1279	rBV2	304418	765206	100.00%	13.573%
9	5.622	1412	1425	1456	rBV	188574	389990	50.97%	6.917%
10	5.912	1506	1515	1534	rBV7	9335	20083	2.62%	0.356%
11	6.072	1552	1565	1590	rBV	179933	367876	48.08%	6.525%
12	6.989	1839	1850	1874	rBV	68884	133356	17.43%	2.365%
13	7.317	1940	1952	1973	rBV	337358	588519	76.91%	10.439%
14	7.400	1973	1978	1989	rVB3	4477	8312	1.09%	0.147%
15	7.625	2038	2048	2068	rBV2	40069	73150	9.56%	1.297%
16	8.092	2183	2193	2237	rBV2	249266	561603	73.39%	9.961%
17	8.854	2416	2430	2457	rBV	285583	474056	61.95%	8.408%
18	10.217	2839	2854	2875	rBV	109616	176766	23.10%	3.135%
19	11.249	3164	3175	3194	rBV	249787	385731	50.41%	6.842%
20	11.622	3280	3291	3316	rBV	289698	462766	60.48%	8.208%


Sum of corrected areas: 5637852

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026252.D
Acq On : 14 Jun 2022 22:36
Operator : SY/MD
Sample : N3275-04 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

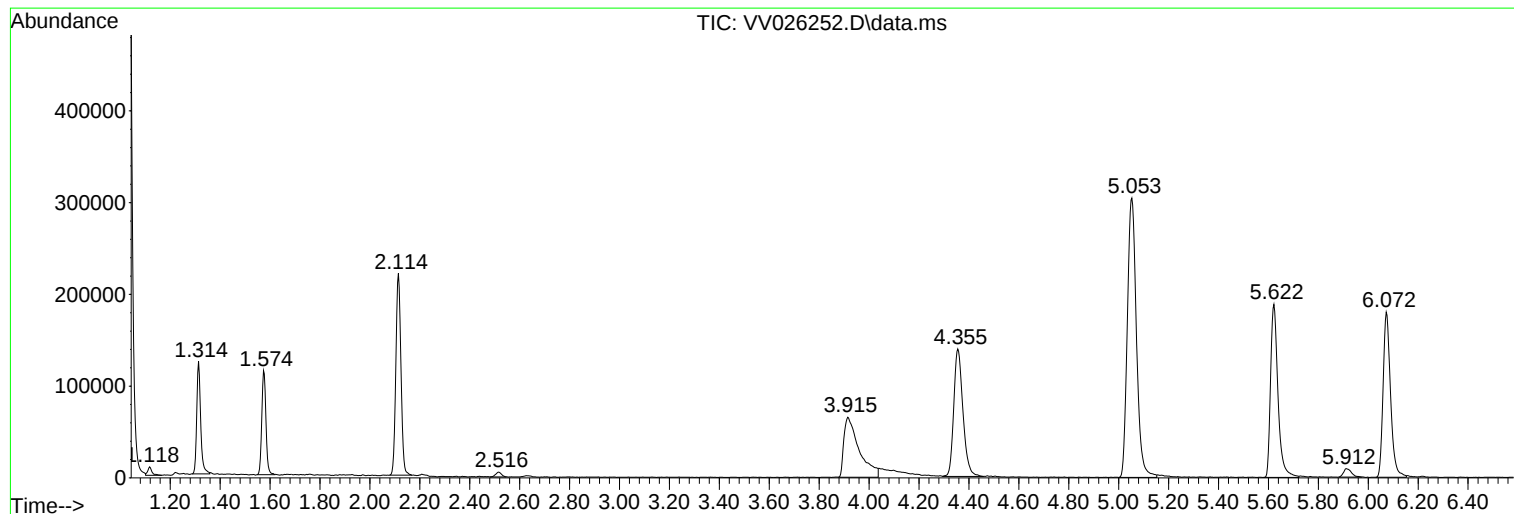

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026252.D
Acq On : 14 Jun 2022 22:36
Operator : SY/MD
Sample : N3275-04 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026252.D
Acq On : 14 Jun 2022 22:36
Operator : SY/MD
Sample : N3275-04 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc