

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026253.D
 Acq On : 14 Jun 2022 23:00
 Operator : SY/MD
 Sample : N3275-05 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026253.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.314	77	85	103	rVB	124576	135477	17.72%	2.423%
2	1.574	157	166	182	rBV	116552	131810	17.24%	2.358%
3	2.114	323	334	352	rVB	220595	316771	41.44%	5.666%
4	2.516	448	459	471	rVB3	5896	9616	1.26%	0.172%
5	3.918	878	895	923	rBV3	74883	302112	39.52%	5.403%
6	4.355	1016	1031	1061	rVB2	138476	352484	46.11%	6.304%
7	5.053	1232	1248	1285	rBV2	306663	764414	100.00%	13.672%
8	5.622	1414	1425	1453	rBV	183114	373891	48.91%	6.687%
9	5.918	1505	1517	1530	rBV6	9235	20422	2.67%	0.365%
10	6.072	1551	1565	1591	rBV	178193	362773	47.46%	6.488%
11	6.989	1840	1850	1872	rBV	67288	129339	16.92%	2.313%
12	7.317	1940	1952	1972	rBV	327950	584352	76.44%	10.452%
13	7.397	1972	1977	1990	rVB4	4842	9660	1.26%	0.173%
14	7.625	2039	2048	2065	rBV	39050	70391	9.21%	1.259%
15	8.092	2183	2193	2235	rBV2	238310	545753	71.39%	9.761%
16	8.423	2283	2296	2311	rVB	12057	21174	2.77%	0.379%
17	8.854	2418	2430	2448	rBV	274547	458434	59.97%	8.199%
18	10.217	2842	2854	2869	rBV	107206	171451	22.43%	3.067%
19	11.249	3163	3175	3193	rBV	241354	372684	48.75%	6.666%
20	11.622	3279	3291	3313	rBV	287807	458049	59.92%	8.193%




Sum of corrected areas: 5591057

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026253.D
Acq On : 14 Jun 2022 23:00
Operator : SY/MD
Sample : N3275-05 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

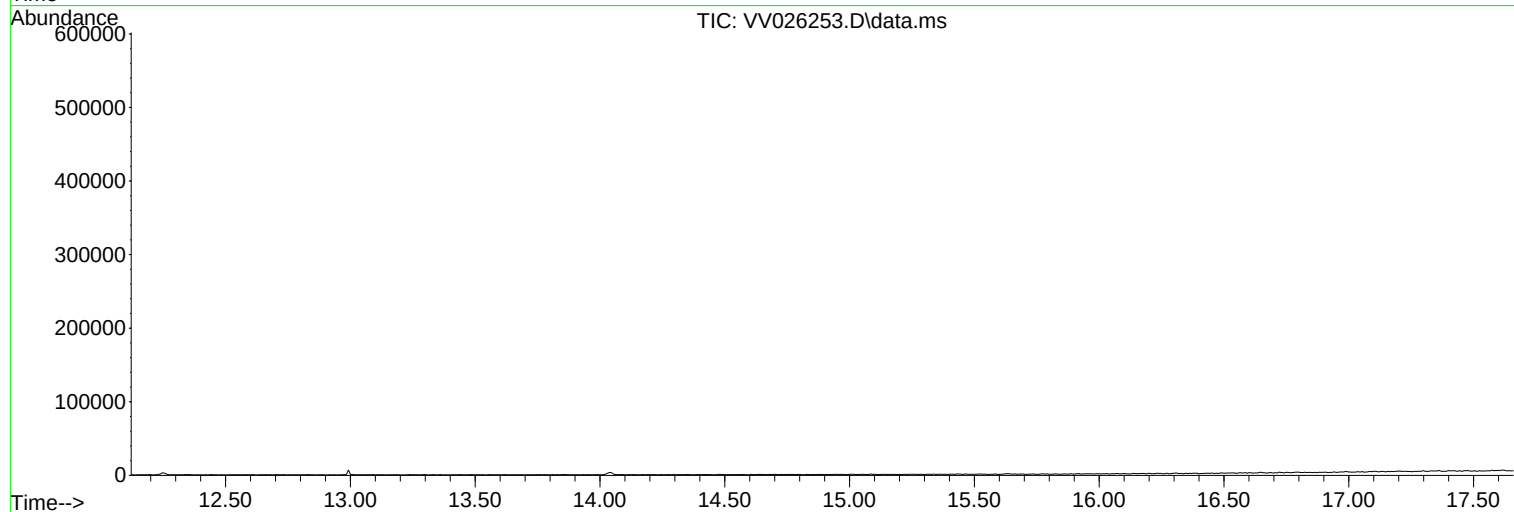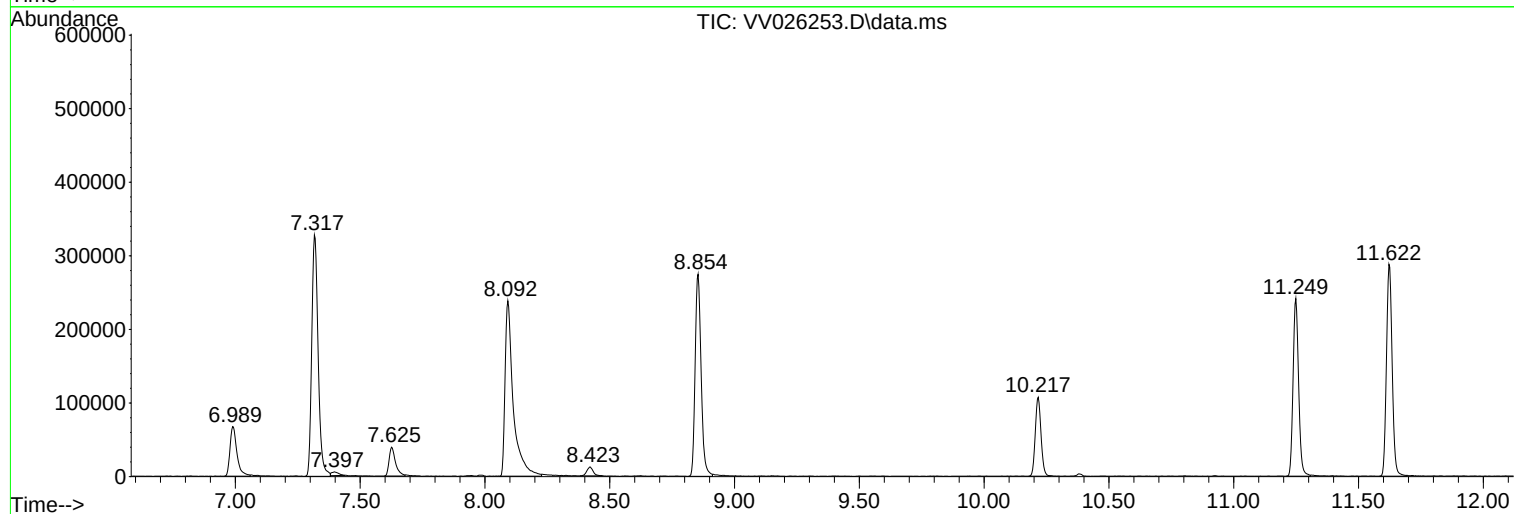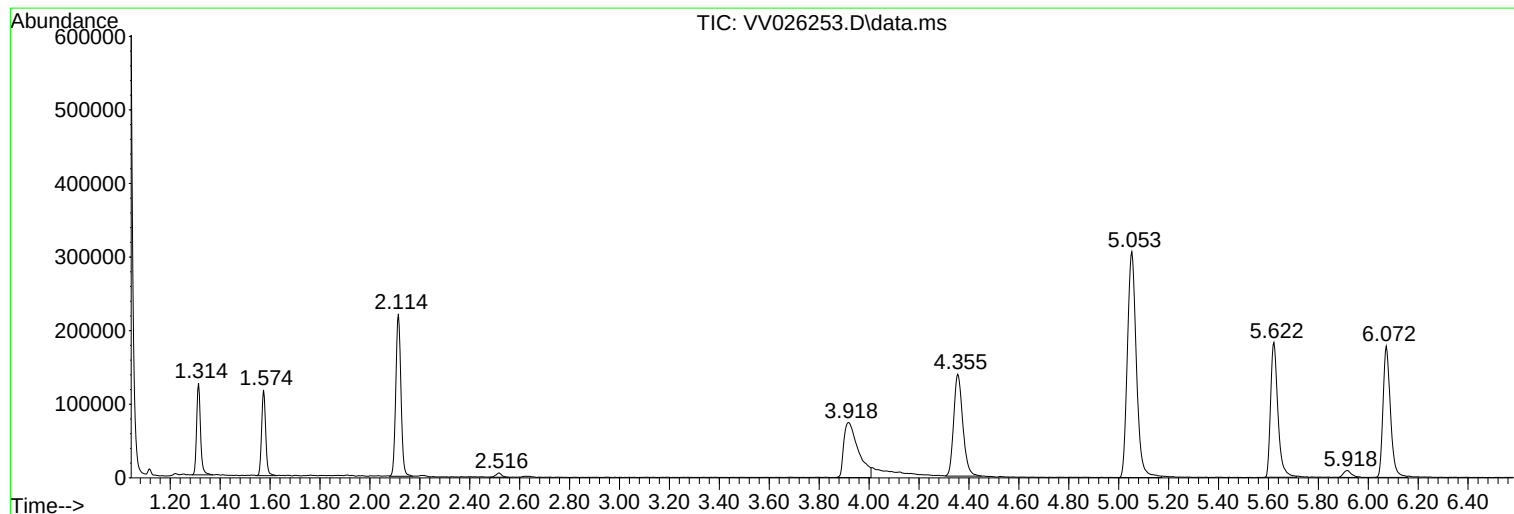

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026253.D
Acq On : 14 Jun 2022 23:00
Operator : SY/MD
Sample : N3275-05 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026253.D
Acq On : 14 Jun 2022 23:00
Operator : SY/MD
Sample : N3275-05 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
