

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026255.D
 Acq On : 14 Jun 2022 23:48
 Operator : SY/MD
 Sample : N3275-07 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026255.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	19	24	41	rVB2	8758	10961	1.43%	0.196%
2	1.314	76	85	99	rBV	124061	134865	17.60%	2.415%
3	1.574	158	166	182	rBV	115969	132236	17.26%	2.368%
4	2.114	322	334	350	rBV	220777	313675	40.93%	5.617%
5	2.516	448	459	468	rBV2	5499	8926	1.16%	0.160%
6	3.912	879	893	928	rBV2	60515	249195	32.52%	4.462%
7	4.355	1015	1031	1069	rVB	139547	358349	46.76%	6.417%
8	5.053	1232	1248	1279	rBV3	303433	766345	100.00%	13.723%
9	5.622	1413	1425	1462	rBV	181390	378769	49.43%	6.783%
10	5.915	1505	1516	1533	rBV5	9141	21389	2.79%	0.383%
11	6.072	1551	1565	1588	rBV	178920	371219	48.44%	6.648%
12	6.989	1840	1850	1883	rBV	68303	131878	17.21%	2.362%
13	7.317	1941	1952	1973	rBV	332357	587769	76.70%	10.525%
14	7.625	2034	2048	2074	rBV	40472	75709	9.88%	1.356%
15	8.092	2182	2193	2234	rBV2	247291	566206	73.88%	10.139%
16	8.854	2415	2430	2455	rBV	275370	460731	60.12%	8.251%
17	10.217	2842	2854	2871	rBV	109037	177130	23.11%	3.172%
18	11.249	3163	3175	3198	rBV	242305	378471	49.39%	6.777%
19	11.622	3280	3291	3309	rBV	289412	460417	60.08%	8.245%




Sum of corrected areas: 5584240

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026255.D
Acq On : 14 Jun 2022 23:48
Operator : SY/MD
Sample : N3275-07 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

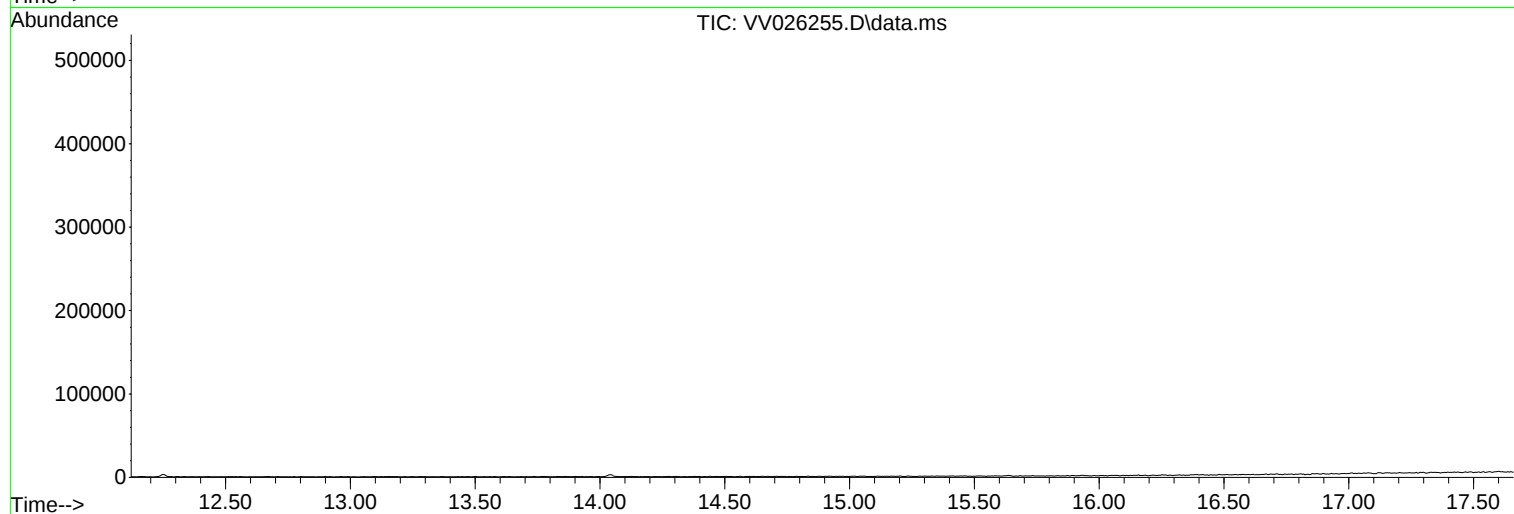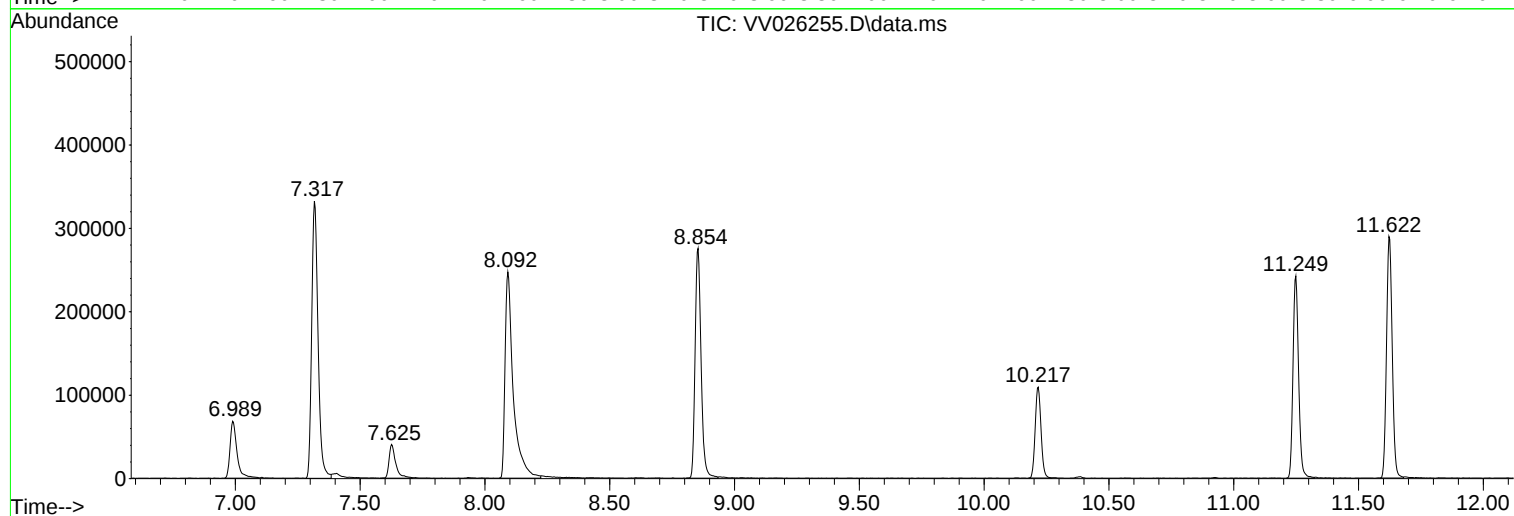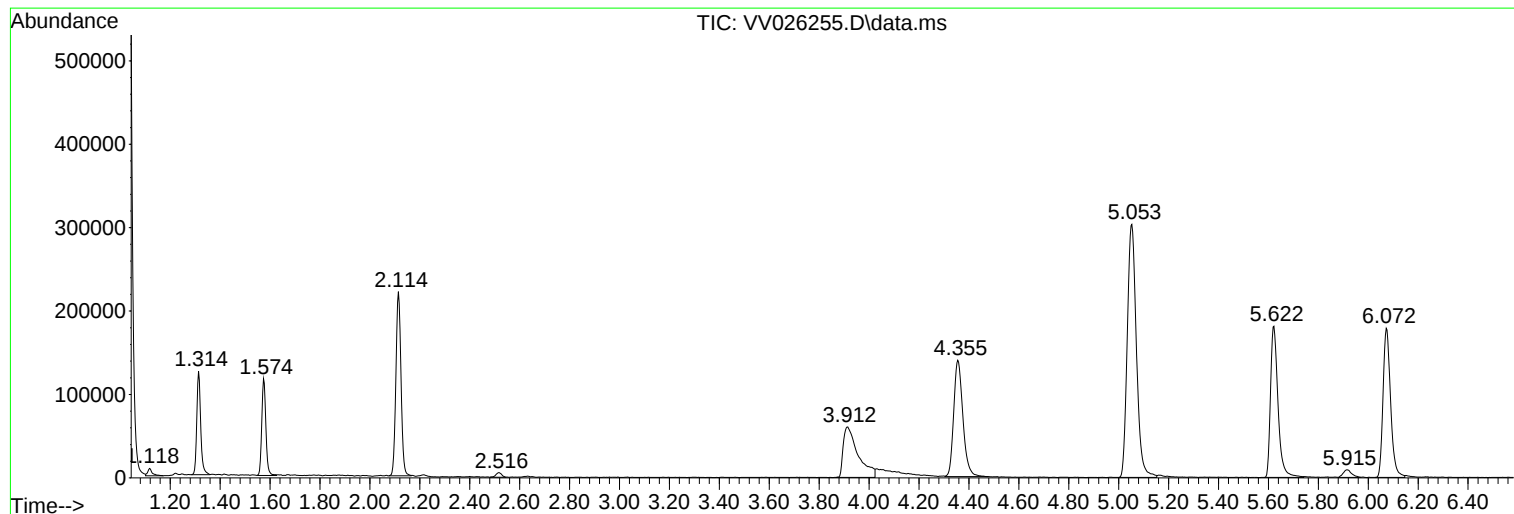

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026255.D
Acq On : 14 Jun 2022 23:48
Operator : SY/MD
Sample : N3275-07 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026255.D
Acq On : 14 Jun 2022 23:48
Operator : SY/MD
Sample : N3275-07 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc