

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026256.D
 Acq On : 15 Jun 2022 00:12
 Operator : SY/MD
 Sample : N3275-08 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026256.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	20	24	31	rVB	8068	7843	1.05%	0.143%
2	1.314	75	85	104	rBV	121141	130721	17.44%	2.378%
3	1.574	158	166	180	rVB	115720	131020	17.48%	2.384%
4	2.114	323	334	350	rVB	215636	308296	41.12%	5.609%
5	2.516	449	459	473	rVB4	5817	10134	1.35%	0.184%
6	3.915	874	894	933	rBV2	61770	261960	34.94%	4.766%
7	4.355	1015	1031	1061	rVB	136314	350851	46.80%	6.383%
8	5.053	1232	1248	1275	rBV3	301817	749667	100.00%	13.639%
9	5.622	1413	1425	1450	rBV2	177029	363206	48.45%	6.608%
10	5.912	1505	1515	1537	rVB7	9323	21547	2.87%	0.392%
11	6.072	1551	1565	1594	rBV	176060	366317	48.86%	6.664%
12	6.989	1840	1850	1877	rBV2	68196	130736	17.44%	2.378%
13	7.317	1941	1952	1973	rBV	329378	580350	77.41%	10.558%
14	7.394	1973	1976	1991	rVB2	4312	8436	1.13%	0.153%
15	7.625	2036	2048	2065	rBV	38071	69664	9.29%	1.267%
16	8.092	2181	2193	2240	rBV2	245385	555460	74.09%	10.105%
17	8.854	2418	2430	2461	rBV	275037	451759	60.26%	8.219%
18	10.217	2841	2854	2871	rBV	106584	171698	22.90%	3.124%
19	11.249	3164	3175	3200	rBV	235319	371727	49.59%	6.763%
20	11.622	3277	3291	3310	rBV	286912	455297	60.73%	8.283%




Sum of corrected areas: 5496689

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026256.D
Acq On : 15 Jun 2022 00:12
Operator : SY/MD
Sample : N3275-08 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

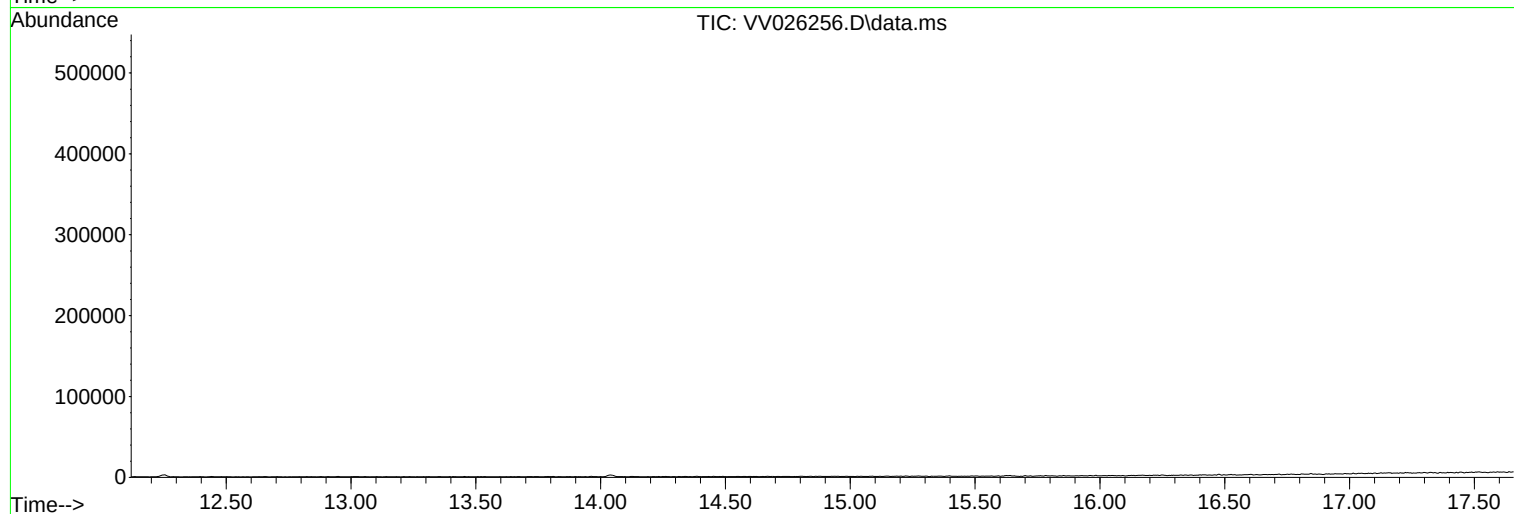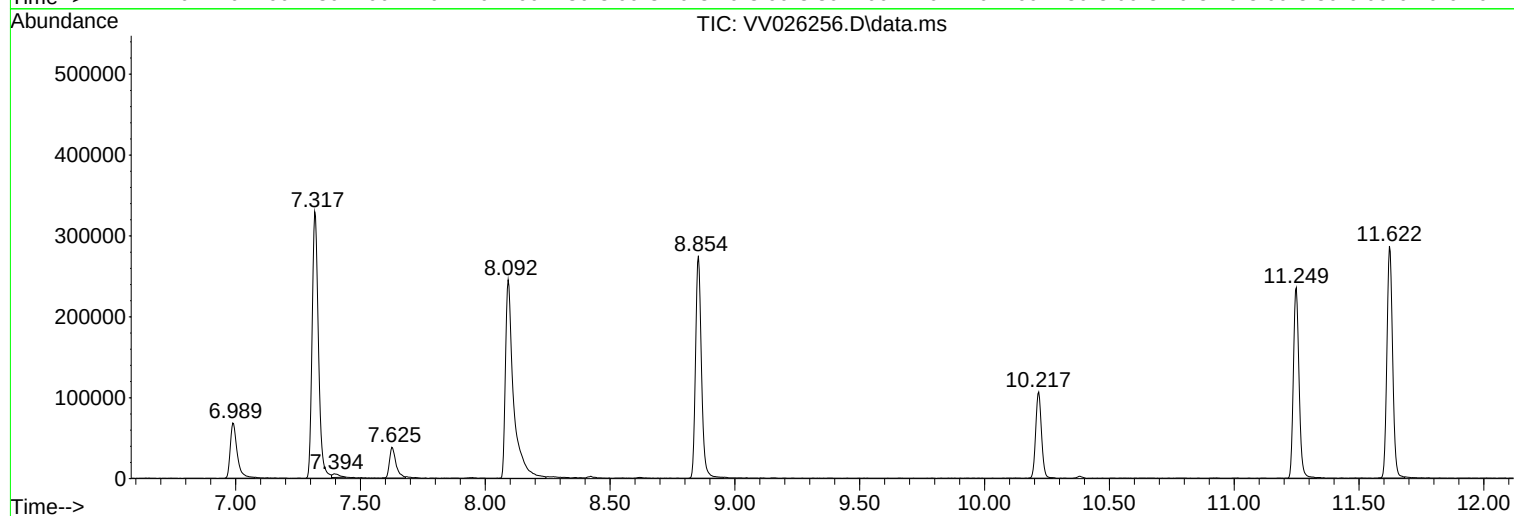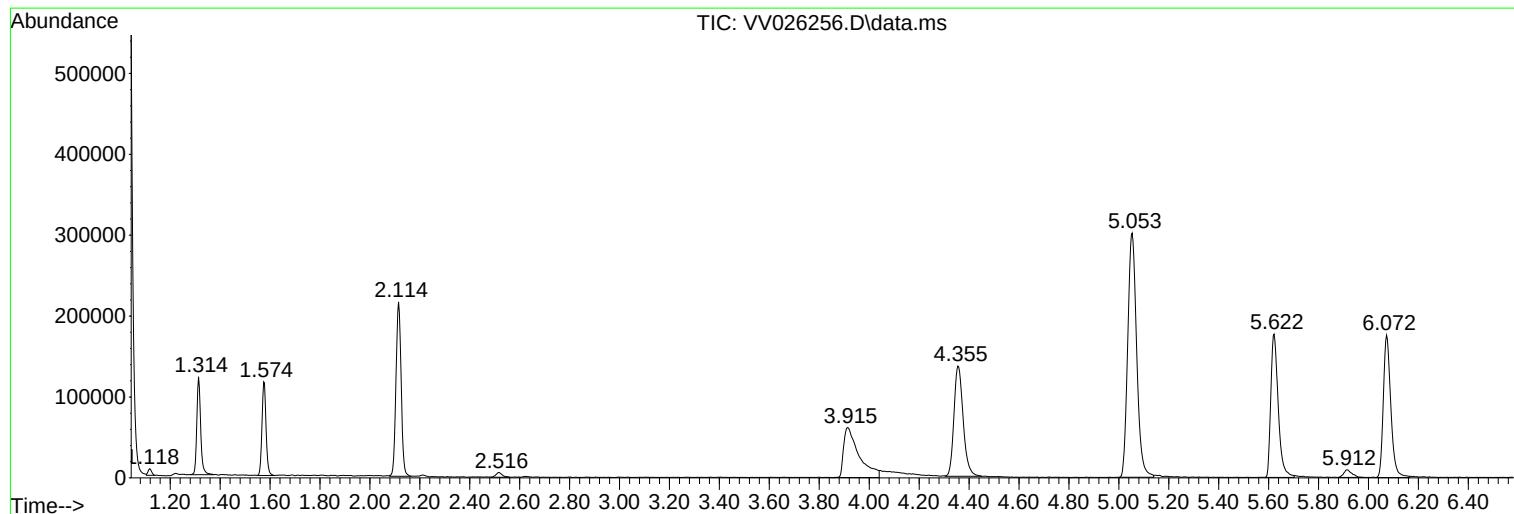

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026256.D
Acq On : 15 Jun 2022 00:12
Operator : SY/MD
Sample : N3275-08 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026256.D
Acq On : 15 Jun 2022 00:12
Operator : SY/MD
Sample : N3275-08 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc