

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026257.D
 Acq On : 15 Jun 2022 00:36
 Operator : SY/MD
 Sample : N3275-09 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026257.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	19	24	40	rVB3	9372	11785	1.51%	0.207%
2	1.314	76	85	106	rVB	124209	135150	17.32%	2.378%
3	1.574	158	166	180	rBV	118061	134879	17.29%	2.374%
4	2.114	322	334	353	rVB	222130	319610	40.96%	5.625%
5	2.516	450	459	469	rVB	6604	10658	1.37%	0.188%
6	3.921	881	896	951	rBV2	58180	319093	40.90%	5.615%
7	4.355	1014	1031	1059	rBV2	139889	360232	46.17%	6.339%
8	5.053	1232	1248	1283	rBV2	311658	780241	100.00%	13.731%
9	5.622	1409	1425	1449	rBV	180574	370932	47.54%	6.528%
10	5.918	1506	1517	1532	rBV7	9164	19950	2.56%	0.351%
11	6.072	1551	1565	1594	rBV	181145	381290	48.87%	6.710%
12	6.989	1839	1850	1873	rBV2	69540	133195	17.07%	2.344%
13	7.317	1939	1952	1972	rBV	337763	599588	76.85%	10.552%
14	7.625	2039	2048	2072	rBV	40736	74315	9.52%	1.308%
15	8.092	2183	2193	2238	rBV2	257141	570597	73.13%	10.041%
16	8.854	2419	2430	2451	rBV	274460	451905	57.92%	7.953%
17	10.217	2839	2854	2872	rBV	110453	178388	22.86%	3.139%
18	11.249	3162	3175	3196	rBV	233357	363578	46.60%	6.398%
19	11.622	3280	3291	3309	rBV	293530	467052	59.86%	8.219%




Sum of corrected areas: 5682438

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026257.D
Acq On : 15 Jun 2022 00:36
Operator : SY/MD
Sample : N3275-09 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

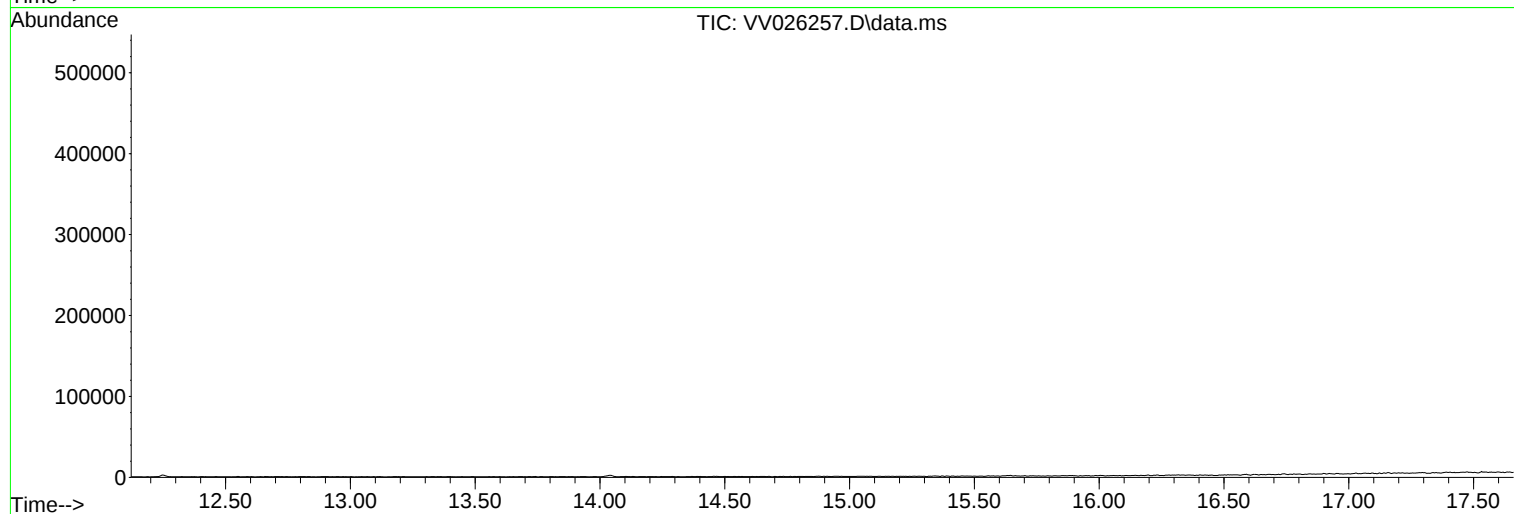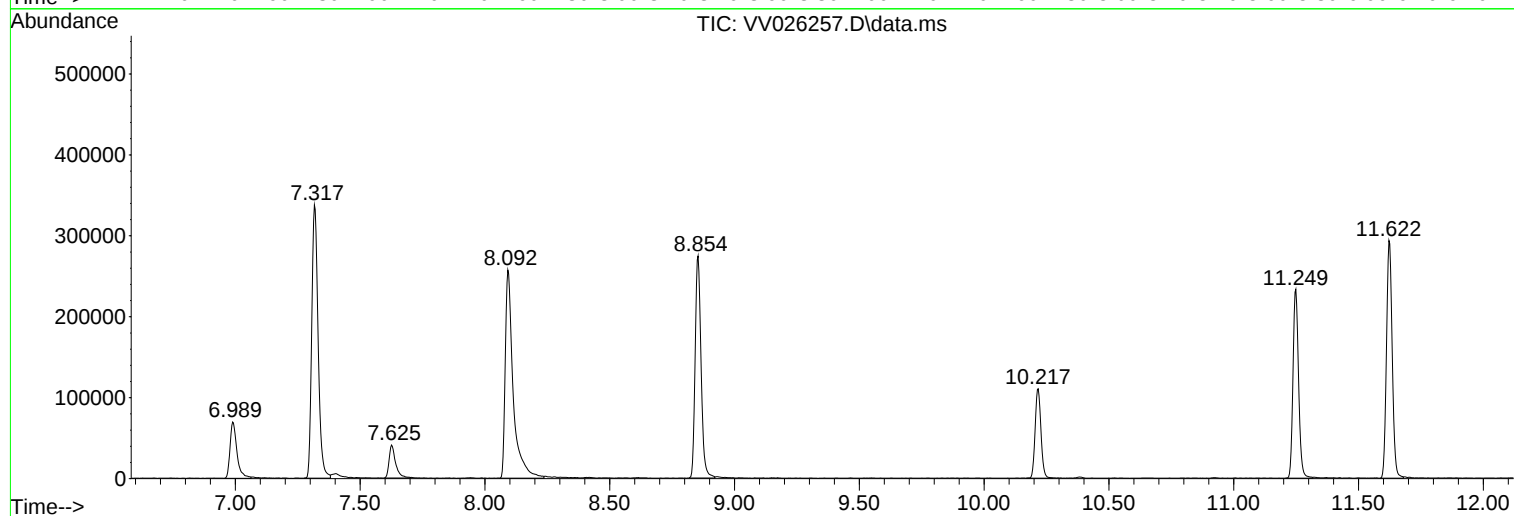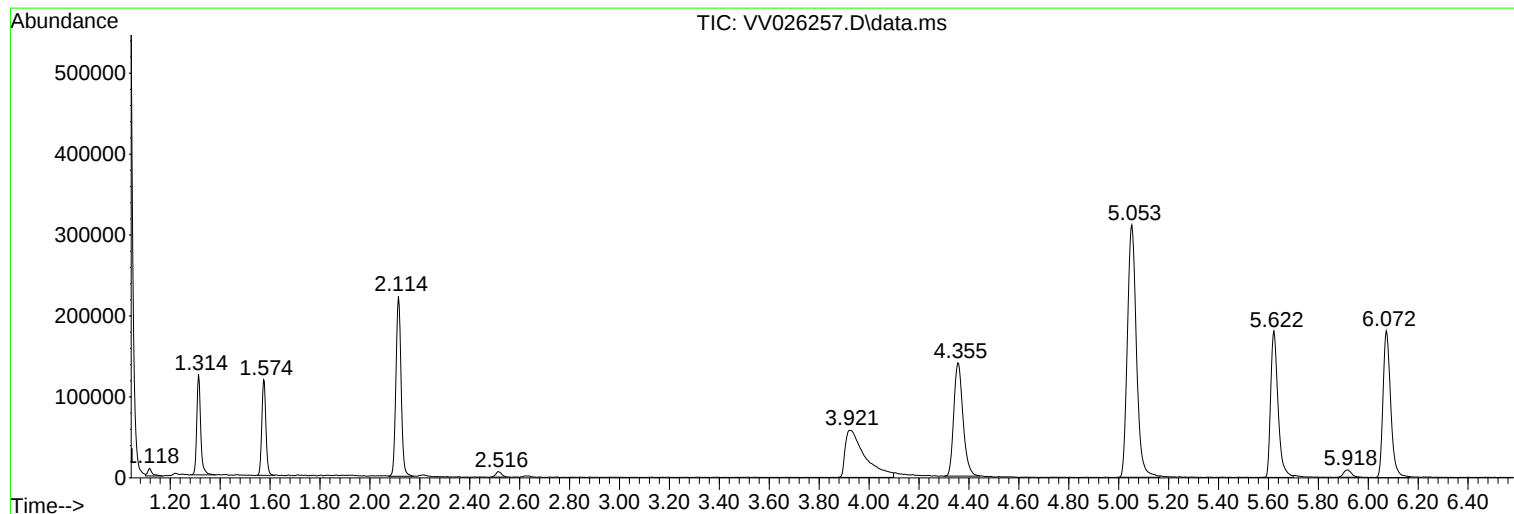

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026257.D
Acq On : 15 Jun 2022 00:36
Operator : SY/MD
Sample : N3275-09 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026257.D
Acq On : 15 Jun 2022 00:36
Operator : SY/MD
Sample : N3275-09 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc