

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026258.D
 Acq On : 15 Jun 2022 01:00
 Operator : SY/MD
 Sample : N3275-10 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026258.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	19	24	32	rVB	7502	7954	1.05%	0.144%
2	1.314	76	85	100	rBV	120834	130354	17.20%	2.352%
3	1.574	158	166	183	rBV	112554	129060	17.03%	2.329%
4	2.114	323	334	351	rVB	211842	306279	40.41%	5.527%
5	2.516	449	459	468	rVB3	6733	11288	1.49%	0.204%
6	3.921	880	896	946	rBV3	58087	294379	38.84%	5.312%
7	4.355	1015	1031	1064	rVB	137488	352732	46.54%	6.365%
8	5.053	1232	1248	1284	rBV3	304997	757836	100.00%	13.674%
9	5.622	1411	1425	1455	rBV	174023	361338	47.68%	6.520%
10	5.918	1499	1517	1536	rBV7	14609	35762	4.72%	0.645%
11	6.072	1552	1565	1587	rBV	175556	361197	47.66%	6.517%
12	6.989	1839	1850	1870	rBV2	65508	127032	16.76%	2.292%
13	7.317	1940	1952	1973	rBV	329435	580843	76.64%	10.481%
14	7.625	2039	2048	2078	rBV	37948	73081	9.64%	1.319%
15	7.979	2148	2158	2174	rVB4	17006	29891	3.94%	0.539%
16	8.092	2182	2193	2230	rBV2	253050	553253	73.00%	9.983%
17	8.854	2418	2430	2451	rBV	259658	436172	57.55%	7.870%
18	10.217	2842	2854	2873	rBV	109199	174106	22.97%	3.142%
19	11.249	3164	3175	3199	rBV	229783	357471	47.17%	6.450%
20	11.625	3279	3292	3309	rBV	287909	461949	60.96%	8.335%




Sum of corrected areas: 5541977

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026258.D
Acq On : 15 Jun 2022 01:00
Operator : SY/MD
Sample : N3275-10 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

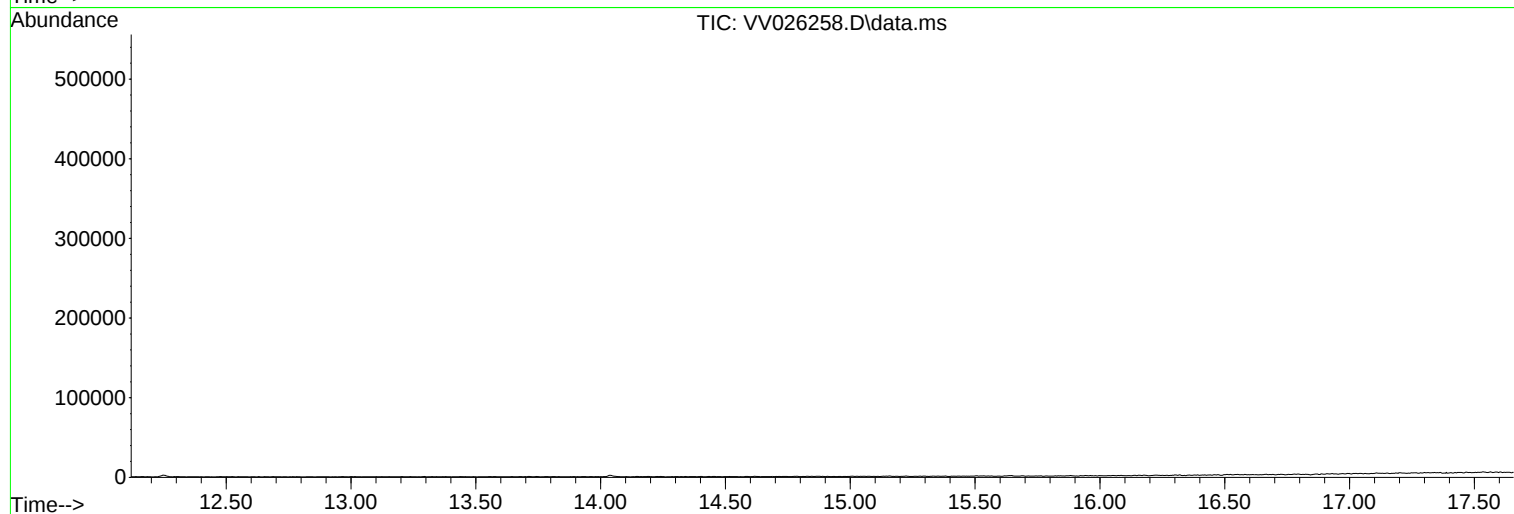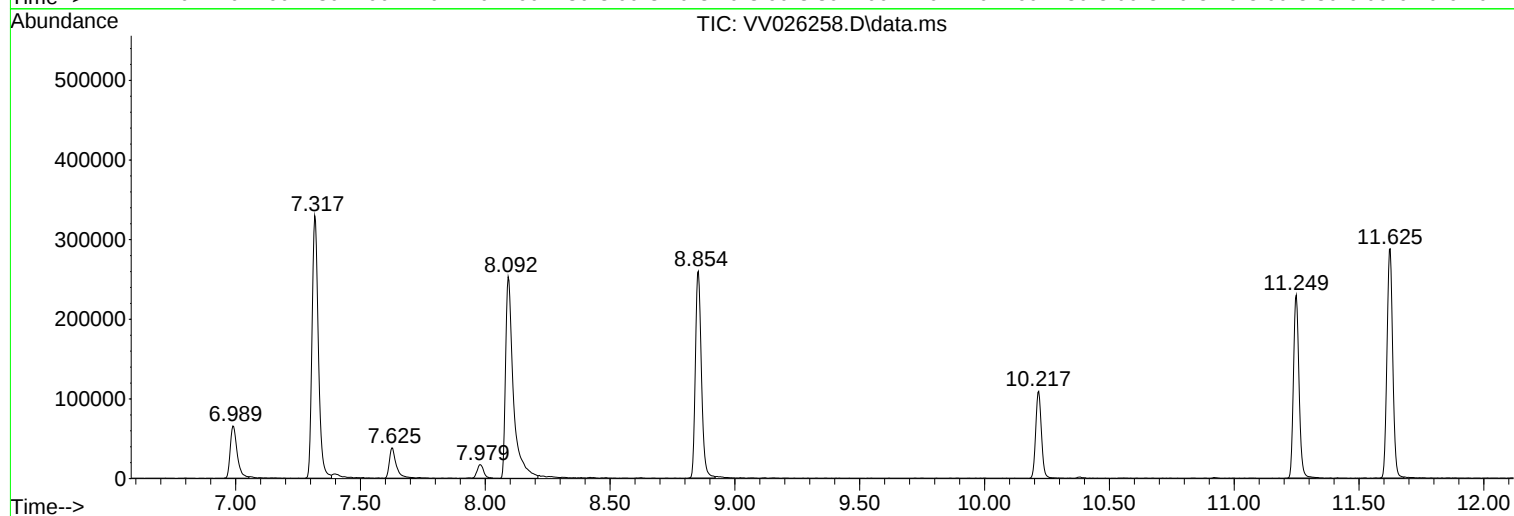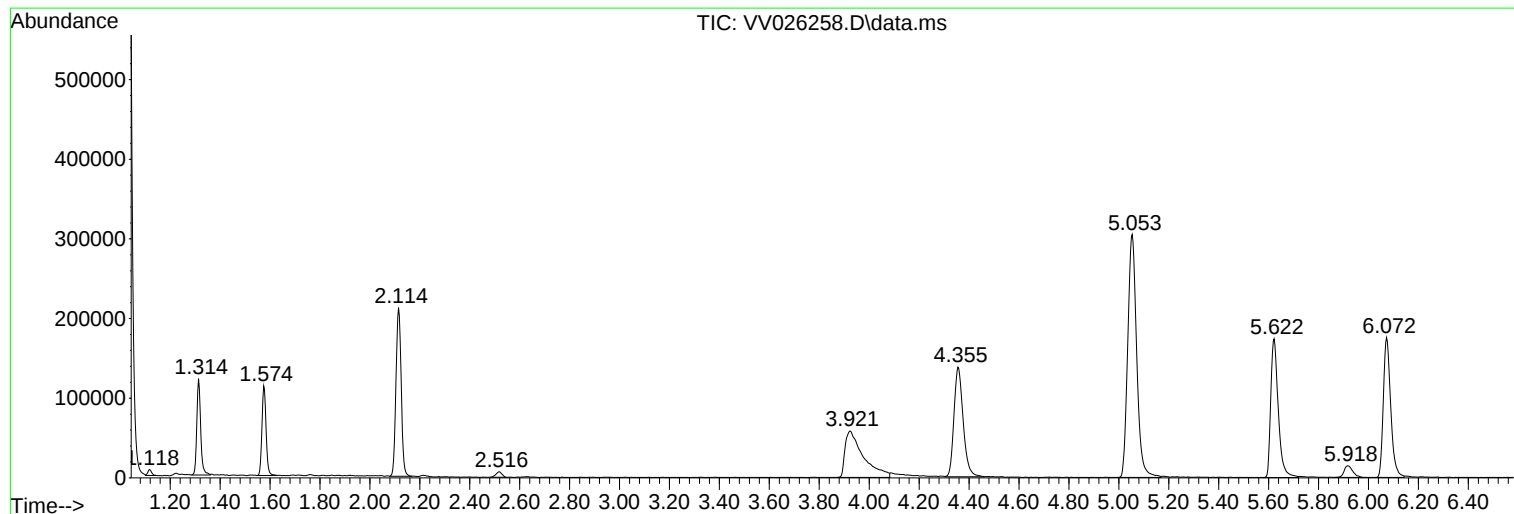

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026258.D
Acq On : 15 Jun 2022 01:00
Operator : SY/MD
Sample : N3275-10 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026258.D
Acq On : 15 Jun 2022 01:00
Operator : SY/MD
Sample : N3275-10 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc