

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026260.D
 Acq On : 15 Jun 2022 01:47
 Operator : SY/MD
 Sample : N3275-12 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026260.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	20	24	39	rVB3	9659	11478	1.50%	0.203%
2	1.314	77	85	105	rVB	125620	132780	17.30%	2.348%
3	1.574	158	166	180	rVB	114688	131914	17.19%	2.333%
4	2.114	323	334	349	rBV	214072	305978	39.87%	5.411%
5	2.516	450	459	472	rVB2	7948	13004	1.69%	0.230%
6	3.918	878	895	934	rBV2	64867	307233	40.03%	5.433%
7	4.355	1015	1031	1058	rBV	140687	354175	46.15%	6.263%
8	5.053	1232	1248	1278	rBV2	305366	767448	100.00%	13.572%
9	5.622	1410	1425	1449	rBV	186130	382808	49.88%	6.770%
10	5.915	1505	1516	1537	rBV7	16675	39621	5.16%	0.701%
11	6.072	1552	1565	1593	rBV	178141	370219	48.24%	6.547%
12	6.989	1840	1850	1877	rBV	67719	131250	17.10%	2.321%
13	7.317	1938	1952	1972	rBV	330109	585109	76.24%	10.347%
14	7.625	2038	2048	2069	rBV	39151	72766	9.48%	1.287%
15	8.092	2182	2193	2231	rBV2	253450	561037	73.10%	9.922%
16	8.854	2418	2430	2452	rBV	282687	467315	60.89%	8.264%
17	10.217	2843	2854	2870	rBV	107953	172312	22.45%	3.047%
18	11.249	3163	3175	3203	rBV	245708	382948	49.90%	6.772%
19	11.622	3279	3291	3319	rBV	296311	465327	60.63%	8.229%




Sum of corrected areas: 5654722

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026260.D
Acq On : 15 Jun 2022 01:47
Operator : SY/MD
Sample : N3275-12 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

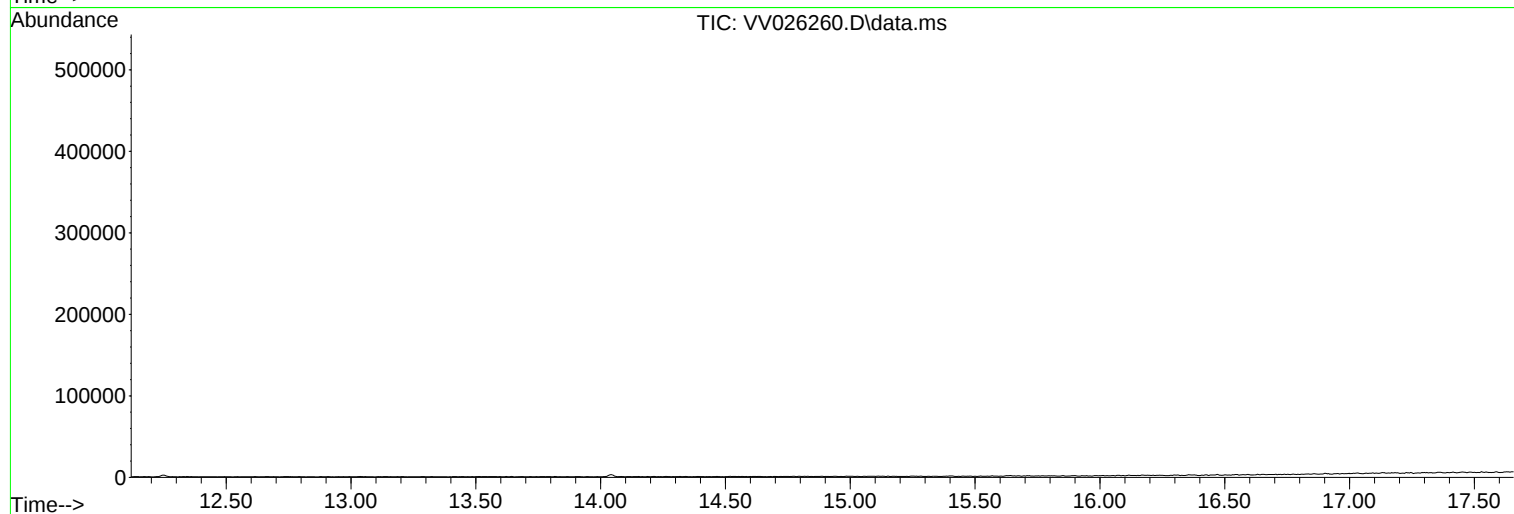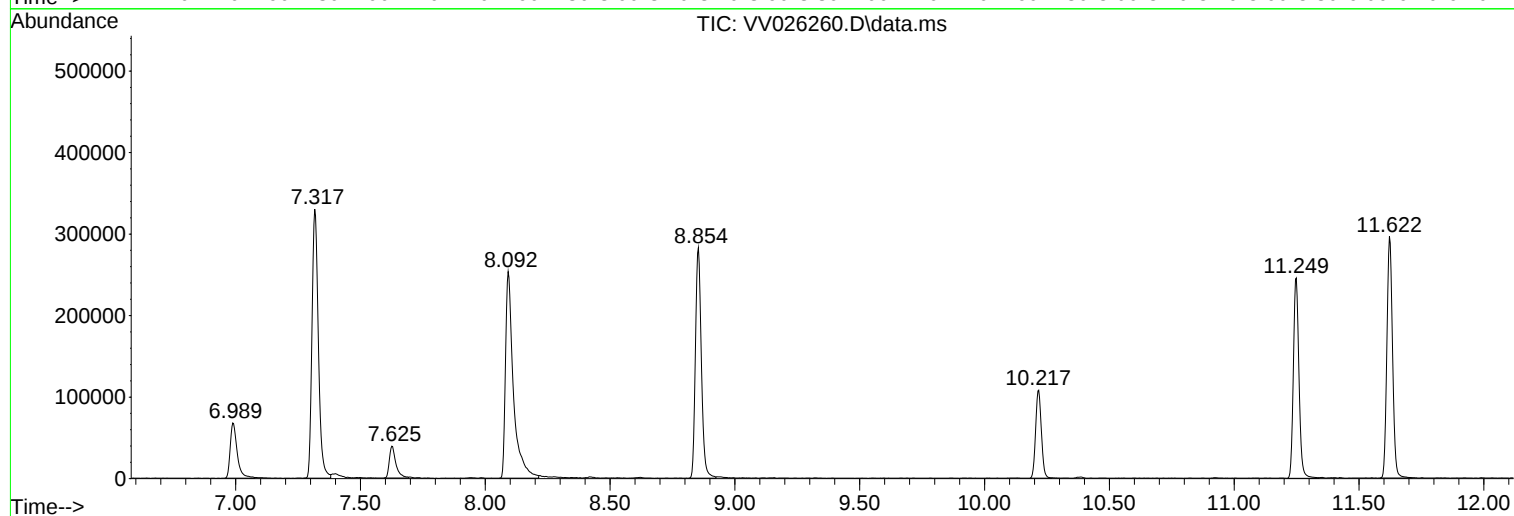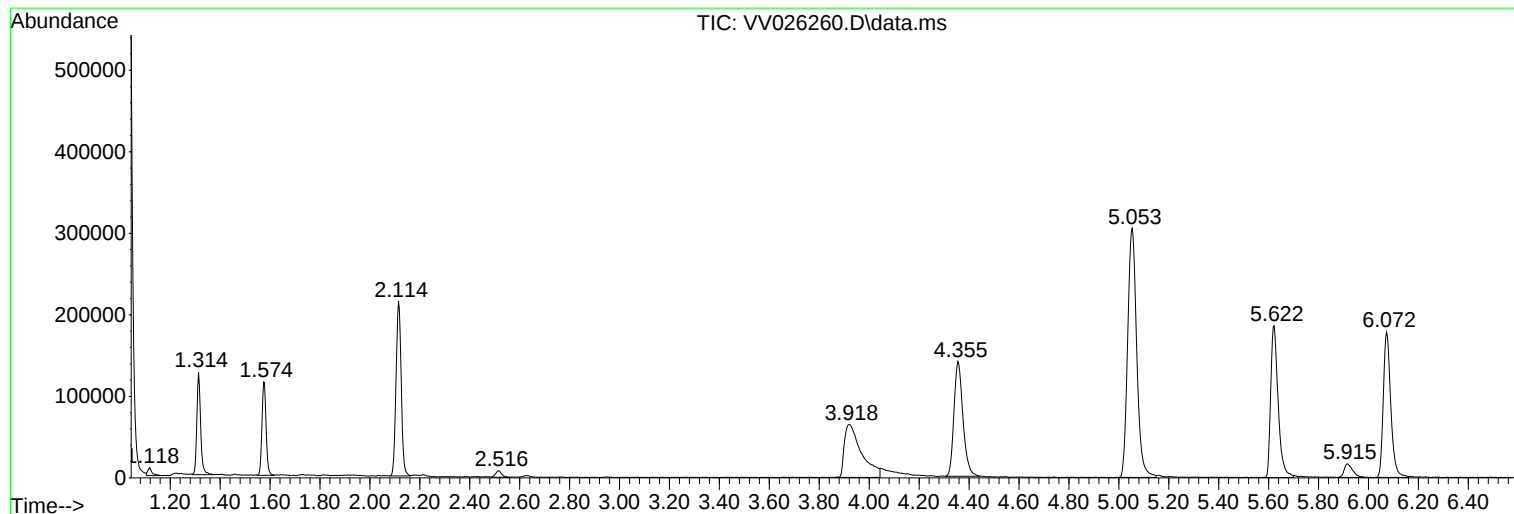

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026260.D
Acq On : 15 Jun 2022 01:47
Operator : SY/MD
Sample : N3275-12 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026260.D
Acq On : 15 Jun 2022 01:47
Operator : SY/MD
Sample : N3275-12 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
