

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026261.D
 Acq On : 15 Jun 2022 02:11
 Operator : SY/MD
 Sample : N3275-13 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026261.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	19	24	37	rVB2	8544	10682	1.38%	0.191%
2	1.314	75	85	106	rVB	123342	134662	17.39%	2.407%
3	1.574	158	166	184	rBV	117120	132710	17.14%	2.372%
4	2.114	323	334	353	rVB	219024	312812	40.40%	5.591%
5	2.516	450	459	469	rBV4	7510	11590	1.50%	0.207%
6	3.915	880	894	933	rBV2	57545	258940	33.45%	4.629%
7	4.355	1015	1031	1060	rVB	141581	359504	46.44%	6.426%
8	5.053	1230	1248	1279	rBV2	313118	774206	100.00%	13.839%
9	5.622	1411	1425	1452	rBV	178099	366266	47.31%	6.547%
10	5.915	1504	1516	1532	rBV4	10219	22089	2.85%	0.395%
11	6.072	1547	1565	1589	rBV	181605	374331	48.35%	6.691%
12	6.989	1839	1850	1881	rBV	68651	133372	17.23%	2.384%
13	7.317	1939	1952	1972	rBV	342069	596010	76.98%	10.654%
14	7.625	2038	2048	2068	rBV	38873	71757	9.27%	1.283%
15	8.092	2183	2193	2229	rBV2	243304	561760	72.56%	10.041%
16	8.854	2418	2430	2452	rBV	271616	451688	58.34%	8.074%
17	10.217	2842	2854	2883	rVB	108278	175720	22.70%	3.141%
18	11.249	3162	3175	3197	rBV	235644	370841	47.90%	6.629%
19	11.622	3280	3291	3315	rBV	311477	475488	61.42%	8.499%




Sum of corrected areas: 5594428

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026261.D
Acq On : 15 Jun 2022 02:11
Operator : SY/MD
Sample : N3275-13 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

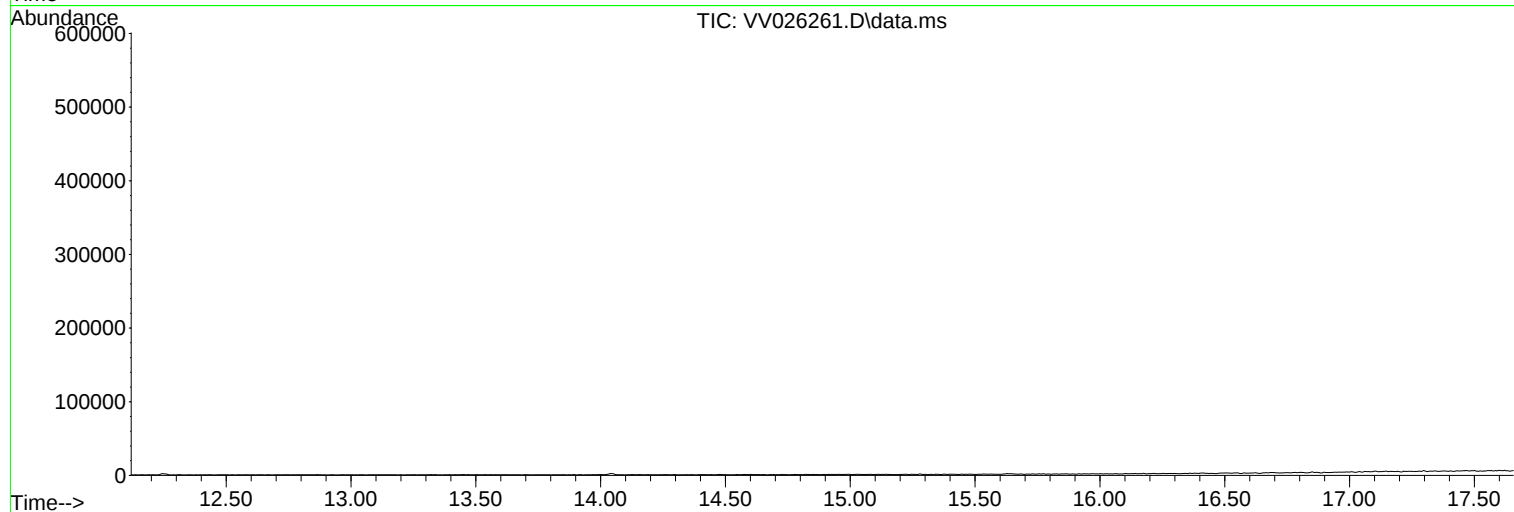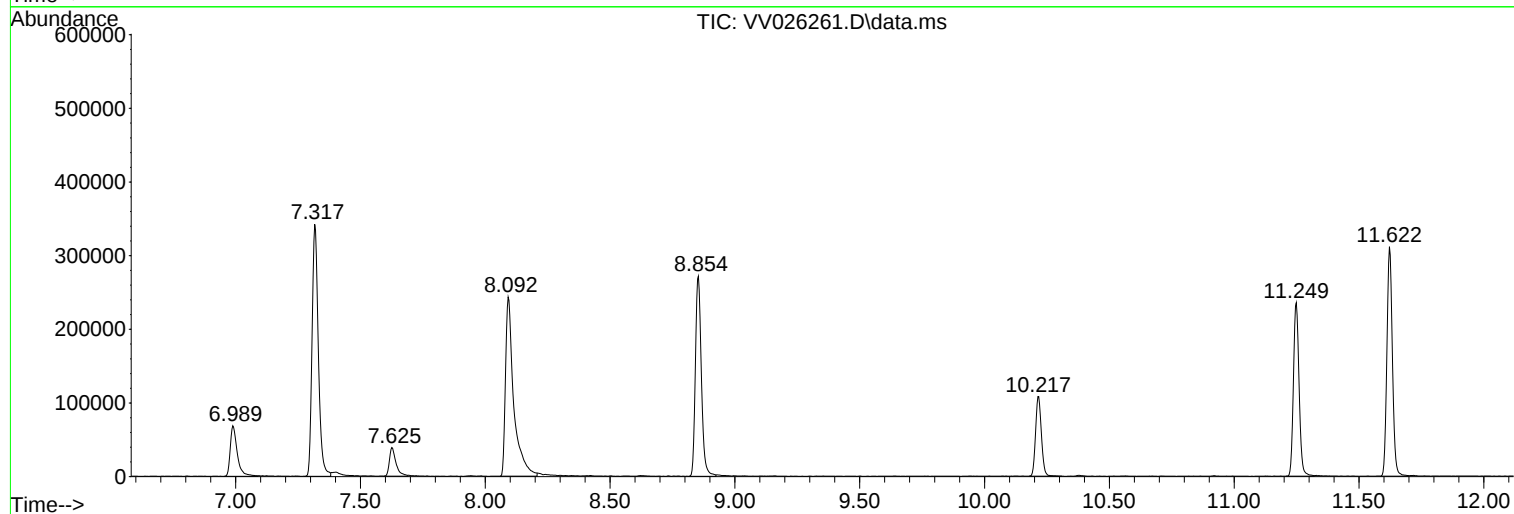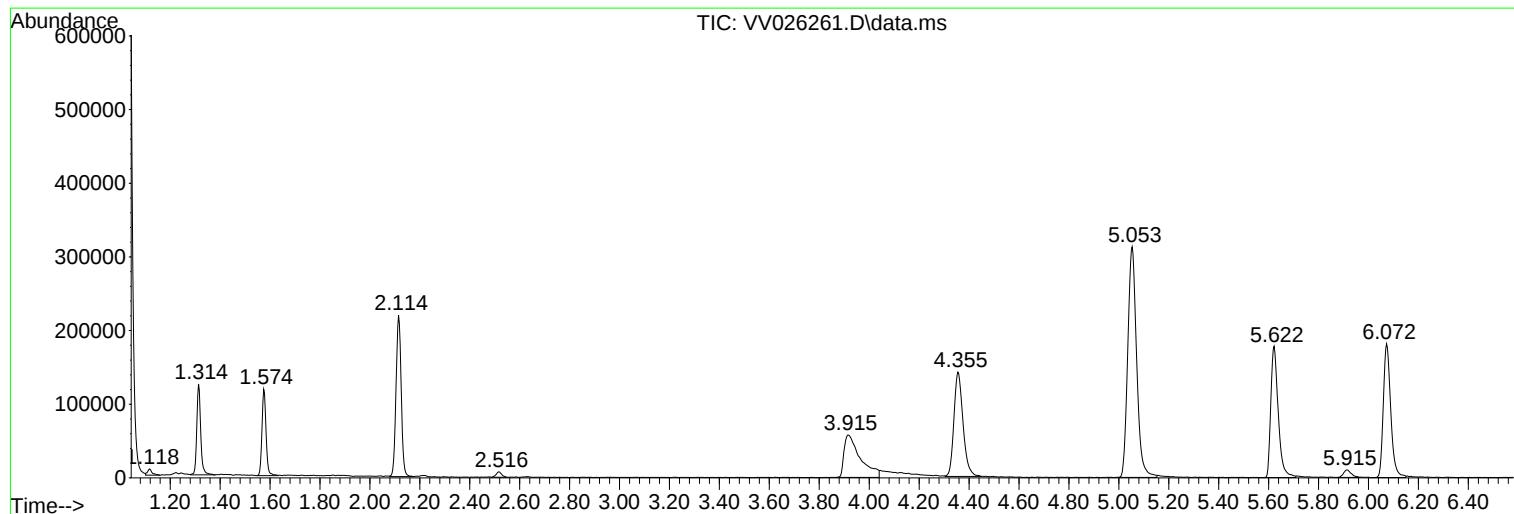

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026261.D
Acq On : 15 Jun 2022 02:11
Operator : SY/MD
Sample : N3275-13 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026261.D
Acq On : 15 Jun 2022 02:11
Operator : SY/MD
Sample : N3275-13 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc