

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026262.D
 Acq On : 15 Jun 2022 02:35
 Operator : SY/MD
 Sample : N3275-14 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026262.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	20	24	36	rVB2	9125	10107	1.28%	0.175%
2	1.314	76	85	105	rVB	126206	134573	17.01%	2.325%
3	1.574	159	166	181	rVB	115657	132698	16.77%	2.293%
4	2.114	323	334	353	rVB	221643	315340	39.85%	5.449%
5	2.516	450	459	469	rBV3	8277	13224	1.67%	0.228%
6	3.918	879	895	937	rBV3	65530	313295	39.60%	5.413%
7	4.355	1015	1031	1061	rVB	142222	365833	46.24%	6.321%
8	5.053	1229	1248	1275	rBV2	319747	791222	100.00%	13.671%
9	5.622	1412	1425	1450	rBV	184418	380374	48.07%	6.572%
10	5.915	1504	1516	1531	rBV5	10624	22548	2.85%	0.390%
11	6.072	1552	1565	1588	rBV	185972	384056	48.54%	6.636%
12	6.989	1840	1850	1880	rBV	70390	134796	17.04%	2.329%
13	7.317	1937	1952	1974	rBV	345144	610196	77.12%	10.543%
14	7.625	2038	2048	2067	rBV	39907	74911	9.47%	1.294%
15	8.092	2181	2193	2236	rBV2	252701	586081	74.07%	10.127%
16	8.854	2417	2430	2452	rBV	278324	469080	59.29%	8.105%
17	10.217	2841	2854	2872	rBV	113732	181324	22.92%	3.133%
18	11.246	3160	3174	3195	rBV	245393	384883	48.64%	6.650%
19	11.622	3280	3291	3313	rBV	304994	482888	61.03%	8.344%




Sum of corrected areas: 5787429

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026262.D
Acq On : 15 Jun 2022 02:35
Operator : SY/MD
Sample : N3275-14 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

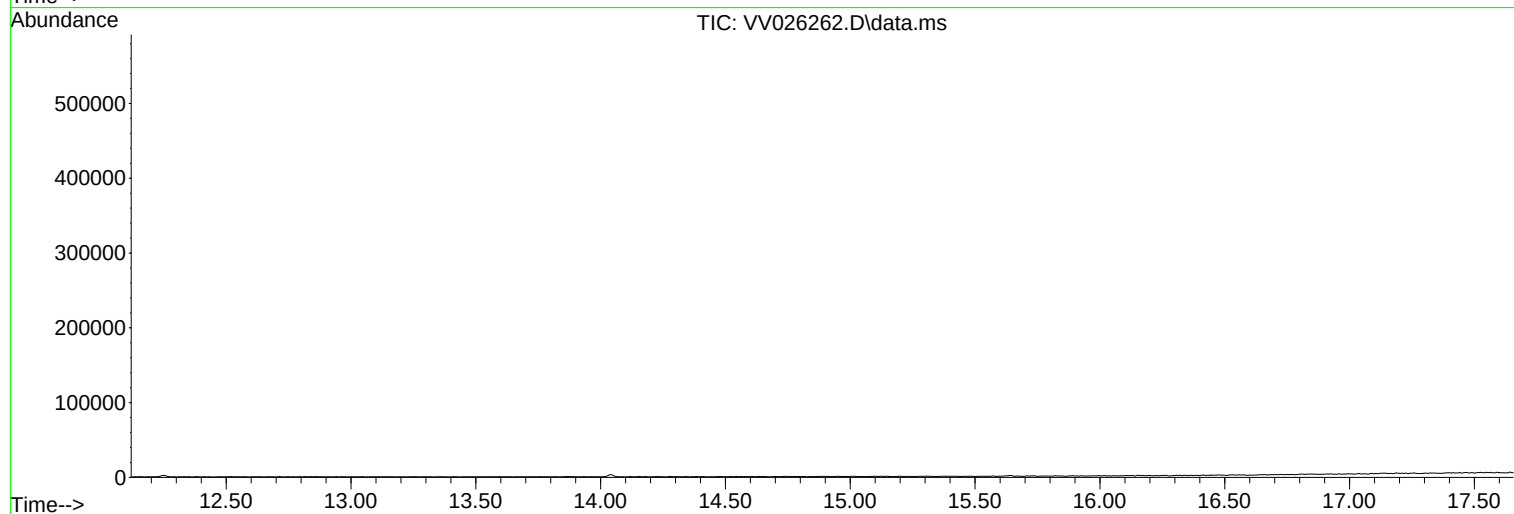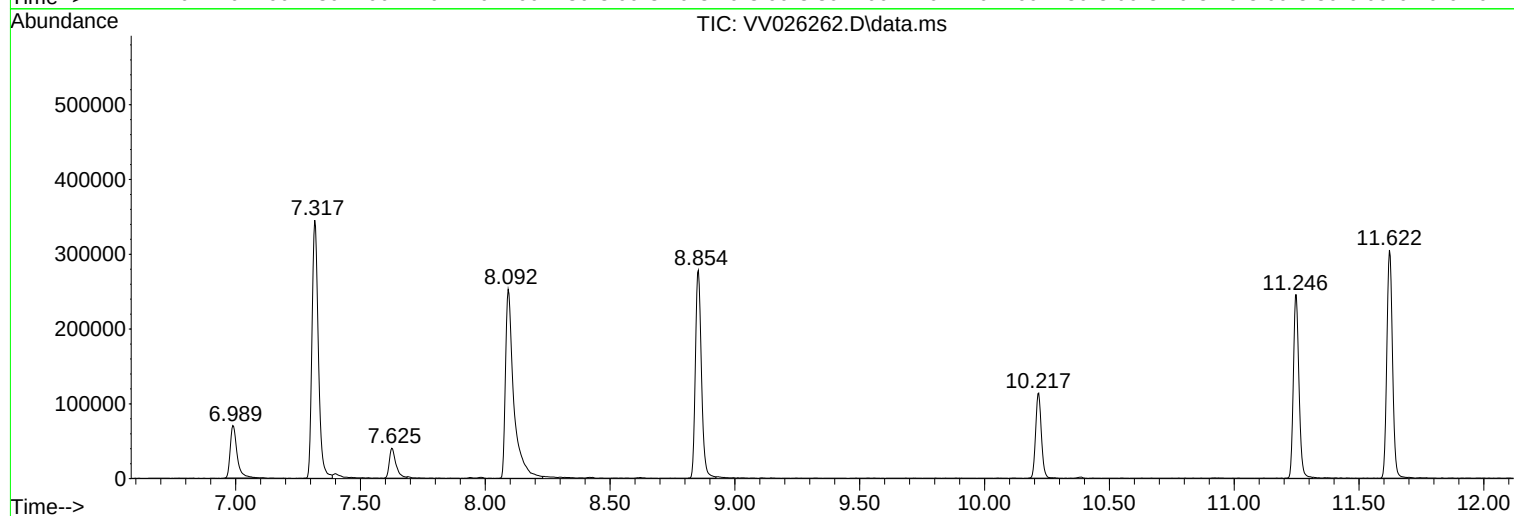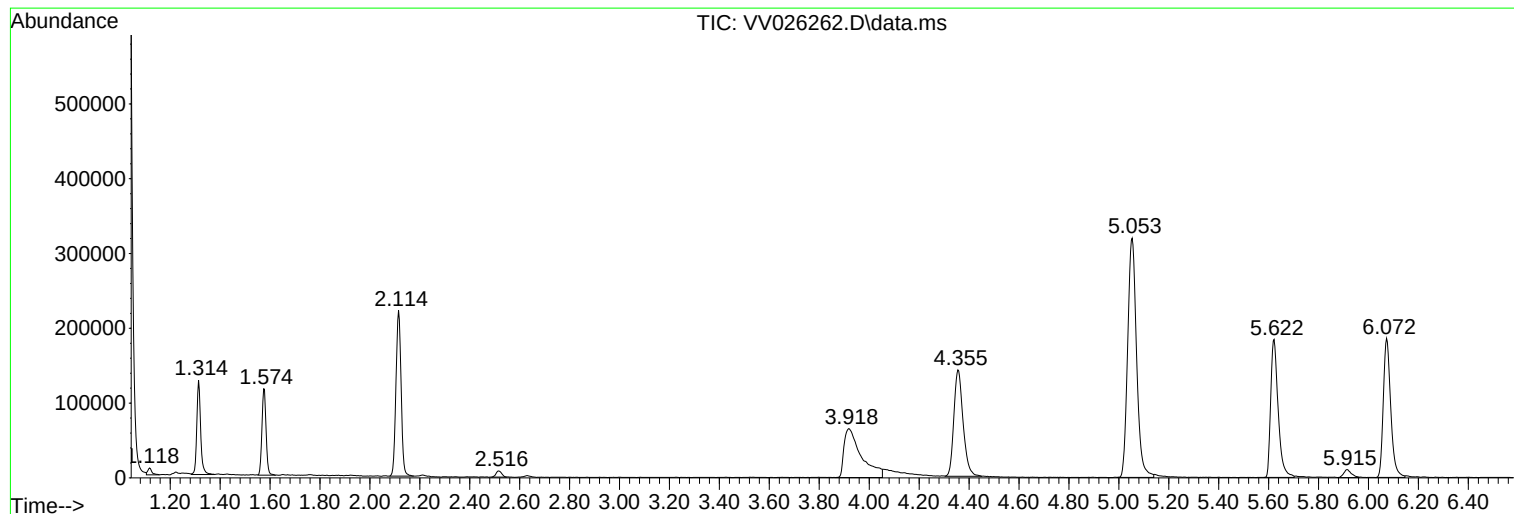

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026262.D
Acq On : 15 Jun 2022 02:35
Operator : SY/MD
Sample : N3275-14 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026262.D
Acq On : 15 Jun 2022 02:35
Operator : SY/MD
Sample : N3275-14 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
