

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026263.D
 Acq On : 15 Jun 2022 02:59
 Operator : SY/MD
 Sample : N3275-15 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026263.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.117	20	24	37	rVB2	9499	10203	1.31%	0.181%
2	1.314	78	85	100	rVB	125532	131657	16.93%	2.334%
3	1.574	158	166	180	rBV	117948	132155	17.00%	2.343%
4	2.114	323	334	352	rVB	214211	308986	39.74%	5.477%
5	2.516	450	459	471	rVB3	9674	15817	2.03%	0.280%
6	3.918	880	895	922	rBV2	65937	272174	35.01%	4.825%
7	4.355	1015	1031	1063	rVB	141619	359219	46.20%	6.368%
8	5.053	1231	1248	1284	rBV2	307954	777512	100.00%	13.782%
9	5.622	1412	1425	1455	rBV	182764	382650	49.21%	6.783%
10	5.911	1505	1515	1534	rVB4	10071	21924	2.82%	0.389%
11	6.072	1552	1565	1584	rBV	180623	371697	47.81%	6.589%
12	6.989	1840	1850	1880	rBV	67803	133871	17.22%	2.373%
13	7.317	1940	1952	1972	rBV	336205	592179	76.16%	10.497%
14	7.625	2039	2048	2074	rBV2	38778	73235	9.42%	1.298%
15	8.091	2183	2193	2235	rBV2	244152	565114	72.68%	10.017%
16	8.853	2419	2430	2461	rBV	281148	470203	60.48%	8.335%
17	10.217	2842	2854	2867	rBV	110221	175790	22.61%	3.116%
18	11.249	3163	3175	3193	rBV	244399	381133	49.02%	6.756%
19	11.622	3280	3291	3308	rBV	296277	465923	59.92%	8.259%




Sum of corrected areas: 5641442

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026263.D
Acq On : 15 Jun 2022 02:59
Operator : SY/MD
Sample : N3275-15 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

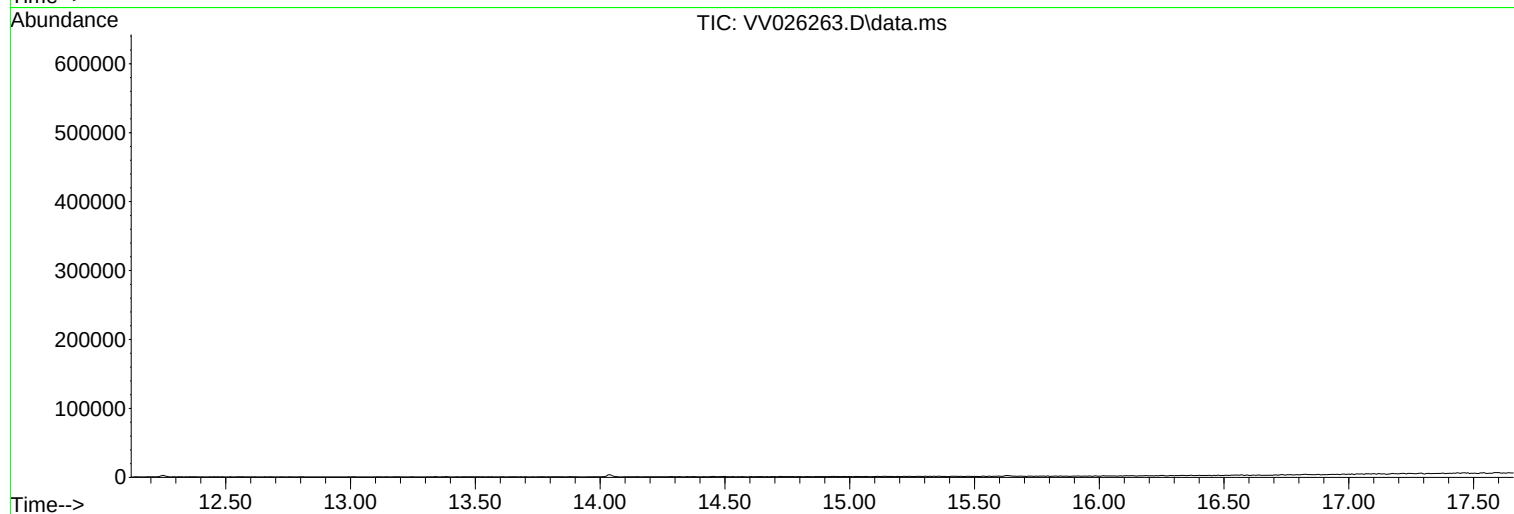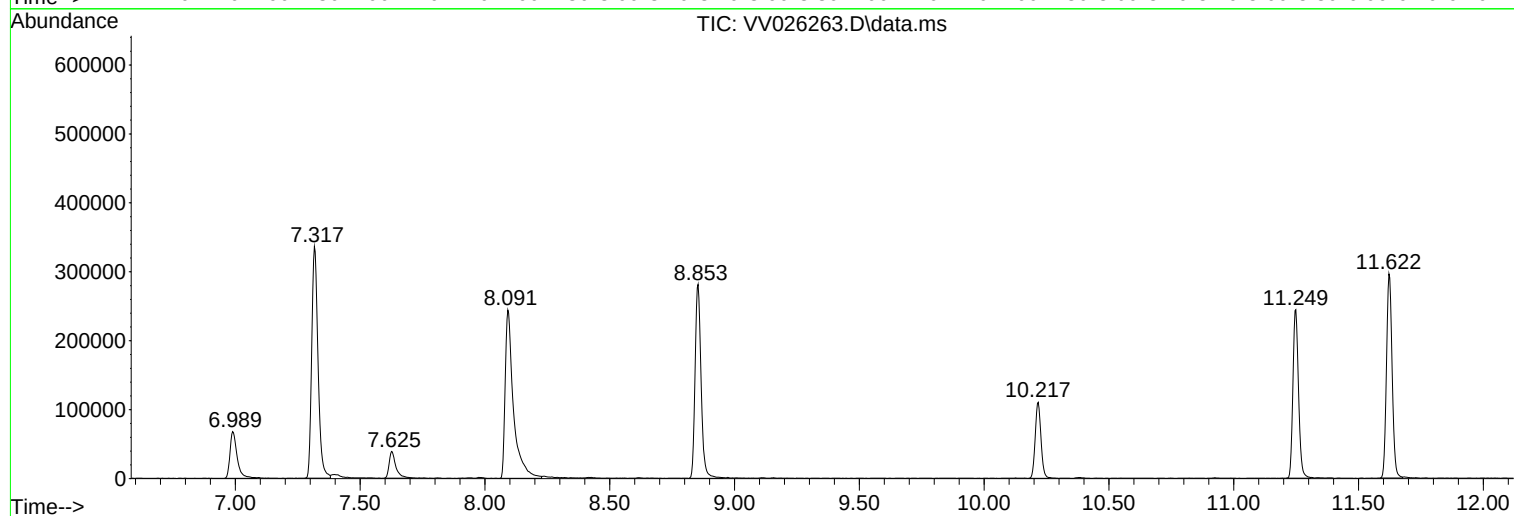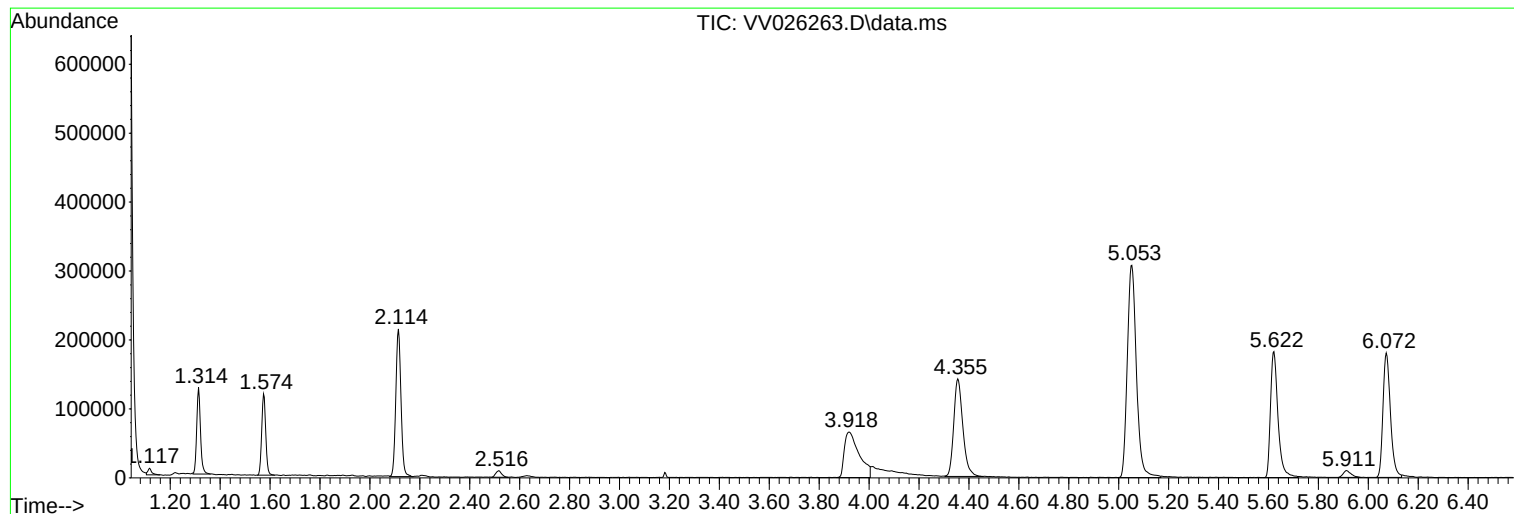

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026263.D
Acq On : 15 Jun 2022 02:59
Operator : SY/MD
Sample : N3275-15 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
Data File : VV026263.D
Acq On : 15 Jun 2022 02:59
Operator : SY/MD
Sample : N3275-15 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc