
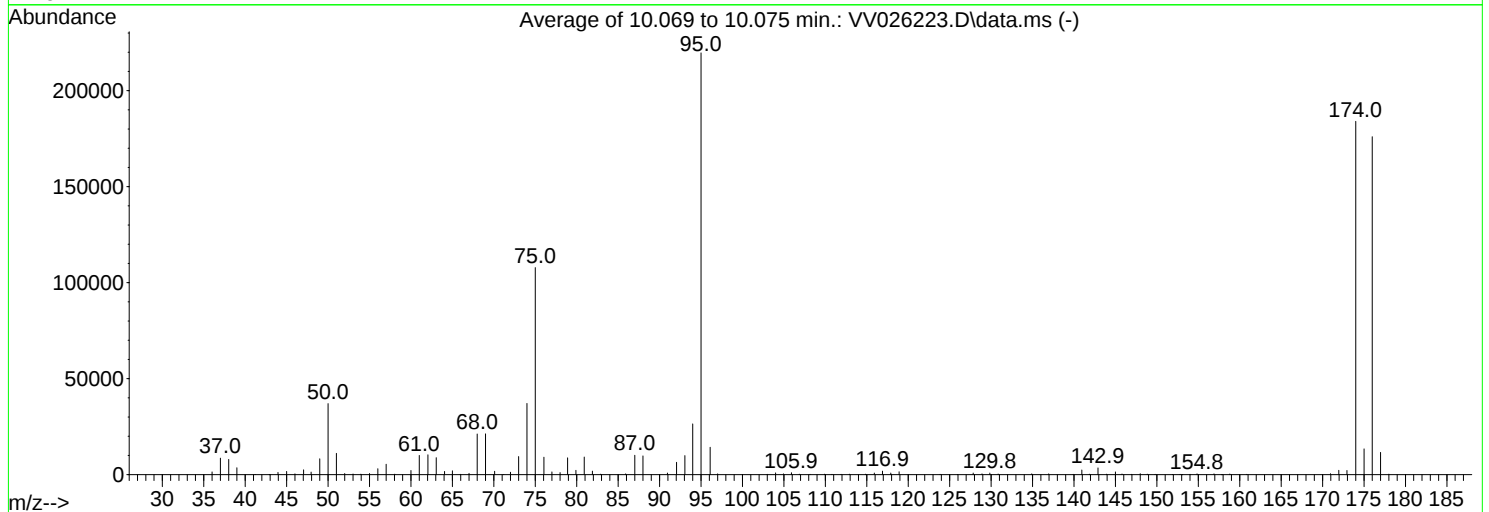


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061422\
 Data File : VV026223.D
 Acq On : 14 Jun 2022 08:58
 Operator : SY/MD
 Sample : BFB328
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB328

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Jun 15 10:58:28 2022

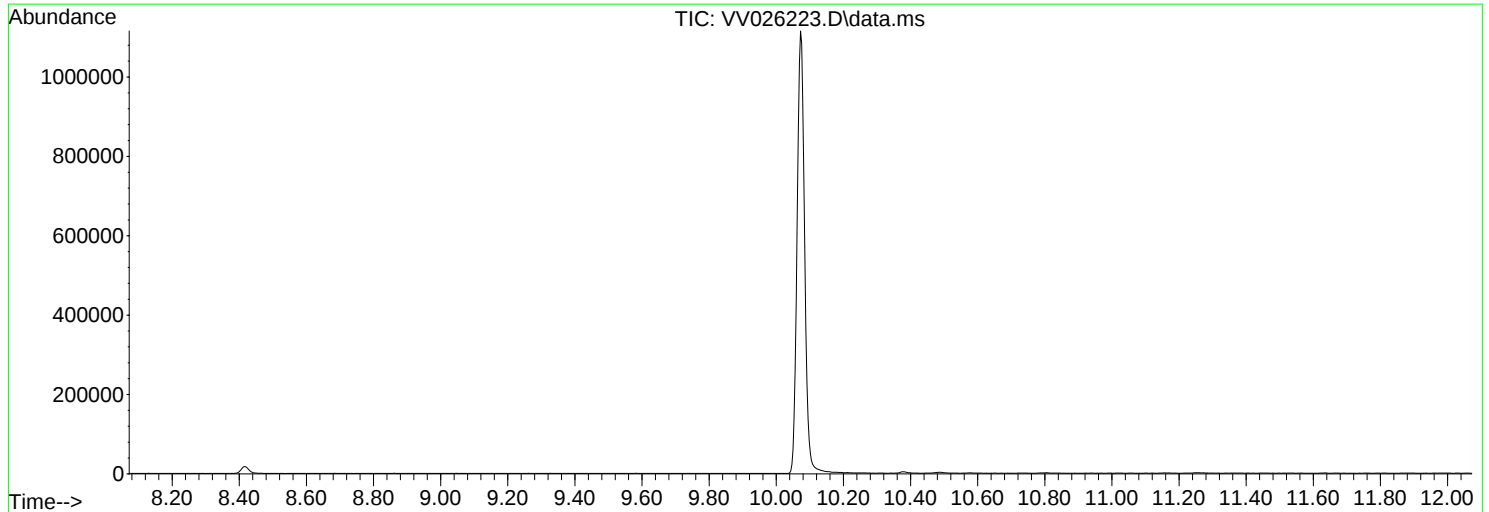

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	36992	PASS
75	95	30	80	49.1	107840	PASS
95	95	100	100	100.0	219648	PASS
96	95	5	9	6.5	14294	PASS
173	174	0.00	2	1.2	2143	PASS
174	95	50	120	83.7	183936	PASS
175	174	5	9	7.3	13380	PASS
176	174	95	105	95.7	176000	PASS
177	176	5	10	6.6	11626	PASS

m/z	Abundance
39.90	1117.0
43.90	257.0

Instrument :
MSVOA_V
ClientSampleId :
BFB328

m/z	Abundance
36.00	1465.0
37.00	8168.0
38.00	7890.0
39.00	3667.0
40.00	1137.0
41.20	126.0
44.00	1266.0
45.00	1629.0
46.00	381.0
47.00	2386.0
47.90	1304.0
49.00	8176.0
50.00	35912.0
51.00	10849.0
52.00	534.0
53.00	285.0
53.90	219.0
55.00	529.0
56.00	2952.0
57.00	5405.0
58.00	295.0
60.00	1976.0
61.00	9578.0
62.10	9733.0
63.10	8753.0
64.10	1632.0
65.00	1886.0
65.90	171.0
67.00	581.0
68.00	20160.0
69.00	21064.0
70.10	1772.0
72.00	1235.0
73.00	9015.0
74.00	35712.0
75.00	104632.0
76.00	8798.0
77.00	1545.0
78.00	1157.0
78.90	8433.0
79.90	2233.0
80.90	8957.0
81.90	1763.0
82.90	202.0
86.00	404.0
87.00	10158.0
88.00	9469.0
90.90	842.0
92.00	6429.0
93.10	9586.0
94.00	25800.0
95.00	211456.0
96.10	13869.0
97.00	481.0
103.00	129.0
104.00	987.0
105.00	382.0
105.90	959.0
106.80	203.0
108.20	176.0
109.90	183.0
110.80	191.0
111.90	188.0
112.90	245.0
114.90	193.0
115.90	759.0
116.90	1749.0
117.90	866.0
118.90	1365.0
123.80	148.0
126.00	114.0
127.80	790.0
128.90	380.0
129.80	782.0
130.90	379.0
134.90	386.0
136.90	427.0
139.90	149.0
141.00	2287.0
141.80	255.0
142.90	3487.0
144.00	247.0
145.00	1486.0
145.80	331.0
146.90	155.0
148.00	466.0
148.90	259.0
149.80	145.0
151.90	109.0
152.80	209.0
154.00	143.0
154.90	425.0

Instrument :
MSVOA_V
ClientSampleId :
BFB328

156.90	393.0
158.70	294.0
160.90	194.0
171.00	463.0
171.90	1981.0
172.90	2086.0
174.00	172544.0
175.00	12988.0
176.00	166656.0
177.00	11196.0
178.00	226.0

Instrument :
MSVOA_V
ClientSampleId :
BFB328

m/z	Abundance
36.00	1532.0
37.00	8915.0
38.00	8180.0
39.00	3718.0
39.90	1075.0
41.20	142.0
44.00	1485.0
45.00	1700.0
46.00	414.0
47.10	2619.0
48.00	1409.0
49.00	8574.0
50.00	38296.0
51.00	11306.0
52.00	591.0
53.00	333.0
54.00	221.0
55.00	589.0
56.00	3191.0
57.00	5509.0
58.00	284.0
60.00	2211.0
61.00	10416.0
62.00	10610.0
63.10	9119.0
64.10	1702.0
65.00	2071.0
66.00	167.0
67.00	692.0
68.00	21864.0
69.00	21824.0
70.10	1798.0
71.20	119.0
72.00	1235.0
73.00	9788.0
74.00	38528.0
75.00	111616.0
76.10	9428.0
77.00	1516.0
78.00	1076.0
78.90	9043.0
79.90	2322.0
80.90	9435.0
81.90	1831.0
82.90	224.0
85.90	387.0
87.00	10470.0
88.00	10170.0
90.90	880.0
92.00	6607.0
93.00	10299.0
94.00	27136.0
95.00	227392.0
96.10	14768.0
97.00	477.0
103.00	152.0
104.00	980.0
105.00	439.0
105.90	1023.0
106.80	256.0
108.10	180.0
109.90	234.0
110.80	197.0
111.90	170.0
112.90	297.0
114.80	250.0
115.90	880.0
116.90	1970.0
117.90	904.0
118.90	1536.0
123.80	170.0
125.90	135.0
127.80	842.0
128.90	431.0
129.90	886.0
130.90	376.0
134.90	397.0
137.00	507.0
139.90	156.0
140.90	2556.0
141.90	251.0
142.90	3684.0
144.00	233.0
145.00	1513.0
145.80	315.0
147.00	148.0
148.00	589.0
148.90	217.0
149.80	164.0
151.90	106.0
152.80	181.0
154.00	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB328

154.80	434.0
156.90	429.0
158.80	321.0
160.80	205.0
170.90	525.0
172.00	2318.0
173.00	2163.0
174.00	190464.0
175.00	13768.0
176.00	182080.0
177.00	12071.0
178.00	258.0

Instrument :
MSVOA_V
ClientSampleId :
BFB328

m/z	Abundance
36.00	1386.0
37.00	8811.0
38.00	7608.0
39.00	3459.0
39.90	1114.0
41.20	113.0
42.90	136.0
44.00	1544.0
45.00	1587.0
46.00	359.0
47.10	2537.0
48.00	1343.0
49.00	7910.0
50.00	36768.0
51.00	11016.0
52.00	533.0
53.00	345.0
54.00	227.0
55.00	565.0
56.00	3134.0
57.00	5280.0
58.10	239.0
60.00	2208.0
61.00	9968.0
62.00	10610.0
63.00	8625.0
64.00	1592.0
65.00	2121.0
66.00	187.0
67.00	656.0
68.00	21376.0
69.00	20848.0
70.10	1670.0
71.20	132.0
72.00	1205.0
73.00	9535.0
74.00	36928.0
75.00	107272.0
76.10	9076.0
77.00	1324.0
78.00	927.0
78.90	8724.0
79.90	2191.0
80.90	9002.0
81.90	1822.0
82.90	231.0
85.80	376.0
87.00	9524.0
88.00	9689.0
91.00	827.0
92.10	6222.0
93.00	9944.0
94.00	26312.0
95.00	220096.0
96.10	14245.0
97.00	371.0
103.00	118.0
104.00	875.0
104.90	435.0
105.90	1040.0
106.90	258.0
108.10	179.0
109.90	233.0
110.80	216.0
111.90	141.0
112.90	280.0
114.80	262.0
115.90	907.0
116.90	1885.0
117.90	742.0
118.90	1542.0
123.90	162.0
125.90	117.0
127.90	780.0
128.90	494.0
129.90	798.0
130.80	369.0
134.90	410.0
137.00	454.0
139.90	132.0
140.90	2471.0
141.90	225.0
142.90	3422.0
143.90	182.0
145.00	1333.0
145.80	260.0
147.00	128.0
148.00	572.0
148.80	176.0
149.80	194.0
152.80	129.0
153.00	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB328

154.00	190.0
154.90	437.0
156.90	388.0
157.80	132.0
158.90	320.0
160.80	224.0
170.90	526.0
172.00	2357.0
173.00	2179.0
174.00	188800.0
175.00	13383.0
176.00	179264.0
177.00	11611.0
178.00	274.0

Instrument :
MSVOA_V
ClientSampleId :
BFB328