


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061423\
Data File : VV031511.D
Acq On : 14 Jun 2023 13:05
Operator : SY/MD
Sample : BFB387
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB387

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Title : VOC Analysis
Last Update : Thu Jun 15 00:30:14 2023

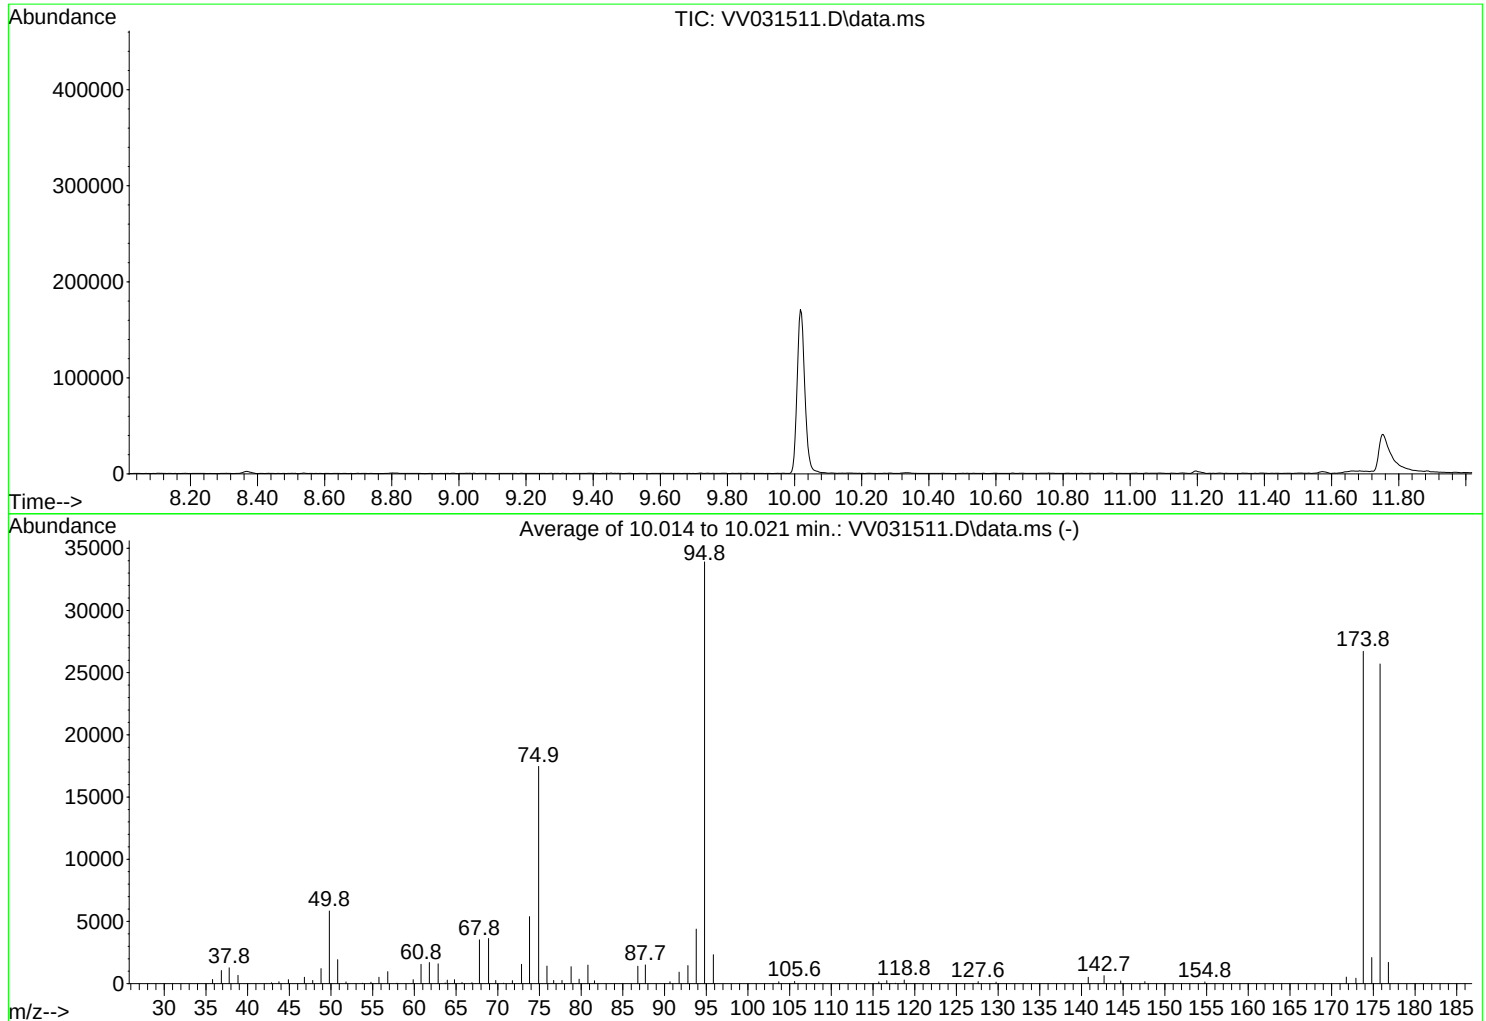

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2781

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	5845	PASS
75	95	30	80	51.5	17467	PASS
95	95	100	100	100.0	33907	PASS
96	95	5	9	6.9	2332	PASS
173	174	0.00	2	1.6	433	PASS
174	95	50	120	78.8	26720	PASS
175	174	5	9	7.9	2101	PASS
176	174	95	105	96.2	25704	PASS
177	176	5	10	6.7	1710	PASS

m/z	Abundance
39.70	157.0
43.80	317.0

Instrument :
MSVOA_V
ClientSampleId :
BFB387

m/z	Abundance
35.80	369.0
36.80	1032.0
37.80	1304.0
38.90	609.0
39.80	171.0
42.90	143.0
43.80	502.0
44.90	326.0
46.80	411.0
47.80	259.0
48.80	1203.0
49.80	5698.0
50.80	1839.0
51.80	150.0
54.70	113.0
55.80	460.0
56.80	973.0
59.90	301.0
60.80	1580.0
61.80	1641.0
62.80	1569.0
63.70	177.0
64.00	189.0
64.80	279.0
67.80	3227.0
68.90	3330.0
69.80	261.0
71.80	228.0
72.80	1513.0
73.80	5639.0
74.90	17312.0
75.90	1449.0
76.70	267.0
77.70	218.0
78.80	1263.0
79.80	364.0
80.80	1392.0
81.60	214.0
86.80	1327.0
87.70	1508.0
90.70	157.0
91.70	926.0
92.80	1372.0
93.80	4235.0
94.80	32896.0
95.90	2209.0
103.70	141.0
105.60	166.0
115.70	123.0
116.80	199.0
118.80	302.0
127.60	166.0
129.80	142.0
140.80	483.0
142.70	640.0
144.70	189.0
147.60	194.0
154.80	157.0
171.70	504.0
172.90	449.0
173.80	24856.0
174.80	1912.0
175.80	24056.0
176.80	1636.0

Instrument :
MSVOA_V
ClientSampleId :
BFB387

m/z	Abundance
35.80	356.0
36.80	1065.0
37.80	1315.0
38.90	702.0
39.80	143.0
42.80	105.0
43.80	484.0
44.90	354.0
46.80	556.0
47.80	265.0
48.80	1262.0
49.80	6023.0
50.80	1964.0
51.80	160.0
54.80	122.0
55.80	500.0
56.80	996.0
57.90	102.0
59.80	340.0
60.80	1598.0
61.80	1737.0
62.80	1709.0
63.90	272.0
64.80	342.0
65.70	113.0
66.90	102.0
67.80	3633.0
68.90	3777.0
69.70	278.0
71.80	268.0
72.90	1624.0
73.80	5506.0
74.90	17992.0
75.90	1448.0
76.70	273.0
77.70	286.0
78.80	1444.0
79.70	375.0
80.80	1547.0
81.60	236.0
86.80	1477.0
87.70	1627.0
90.70	161.0
91.70	952.0
92.80	1492.0
93.80	4527.0
94.80	35080.0
95.80	2402.0
103.70	157.0
105.60	189.0
115.70	140.0
116.60	245.0
117.70	102.0
118.70	304.0
127.60	172.0
129.80	136.0
140.80	524.0
142.70	668.0
144.70	212.0
147.60	164.0
154.80	150.0
171.70	520.0
172.90	444.0
173.80	27592.0
174.80	2168.0
175.80	26424.0
176.80	1717.0

Instrument :
MSVOA_V
ClientSampleId :
BFB387

m/z	Abundance
35.80	296.0
36.90	1058.0
37.80	1207.0
38.80	711.0
39.80	142.0
43.70	447.0
44.90	289.0
46.80	570.0
47.80	234.0
48.80	1168.0
49.80	5815.0
50.80	1999.0
51.80	105.0
53.80	120.0
54.90	114.0
55.70	575.0
56.80	922.0
59.80	346.0
60.80	1484.0
61.80	1709.0
62.90	1526.0
63.90	399.0
64.80	363.0
65.70	147.0
66.90	115.0
67.80	3725.0
68.90	3777.0
69.70	251.0
70.70	112.0
71.70	232.0
72.90	1550.0
73.80	5043.0
74.90	17096.0
75.90	1340.0
76.70	232.0
77.70	280.0
78.80	1401.0
79.70	342.0
80.80	1542.0
81.60	253.0
86.80	1422.0
87.70	1365.0
90.60	146.0
91.80	902.0
92.80	1509.0
93.80	4417.0
94.80	33744.0
95.80	2384.0
103.70	154.0
105.60	194.0
115.70	155.0
116.60	289.0
118.80	291.0
127.60	162.0
129.70	105.0
140.80	549.0
142.70	615.0
144.70	263.0
147.60	134.0
154.80	126.0
171.80	558.0
172.90	407.0
173.80	27712.0
174.80	2224.0
175.80	26632.0
176.80	1777.0

Instrument :
MSVOA_V
ClientSampleId :
BFB387