

Data File : VV006274.D

Acq On : 15 Jun 2018 11:32

Operator : SY/MD

Sample : J3397-08

Misc : 25 mL/MSVOA_V/WATER

ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEXW2

Quant Time: Jun 16 00:05:15 2018

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Fri Jun 15 23:47:49 2018

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	341416	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	306435	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	136552	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	67377	3.61	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.20%
7) Chloroethane-d5	1.59	69	60937	4.08	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.60%
11) 1,1-Dichloroethene-d2	2.13	63	100327	2.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.40%#
20) 2-Butanone-d5	3.98	46	185741	46.91	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.82%
24) Chloroform-d	4.41	84	132919	3.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	73.60%
26) 1,2-Dichloroethane-d4	5.09	65	68275	3.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.20%
32) Benzene-d6	5.11	84	275949	3.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.00%
36) 1,2-Dichloropropane-d6	6.12	67	84324	3.81	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	76.20%
41) Toluene-d8	7.37	98	249922	3.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.20%
43) trans-1,3-Dichloropropene-	7.67	79	26873	2.71	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	54.20%#
46) 2-Hexanone-d5	8.14	63	146928	34.35	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	68.70%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	55991	3.49	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	69.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	94274	3.98	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	79.60%#

Target Compounds


						Qvalue
13) Acetone	2.22	43	7286	3.396	ug/L	79
16) Methylene chloride	2.54	84	34466	1.593	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV006274.D
Acq On : 15 Jun 2018 11:32
Operator : SY/MD
Sample : J3397-08
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEXW2

Quant Time: Jun 16 00:05:15 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 15 23:47:49 2018
Response via : Initial Calibration

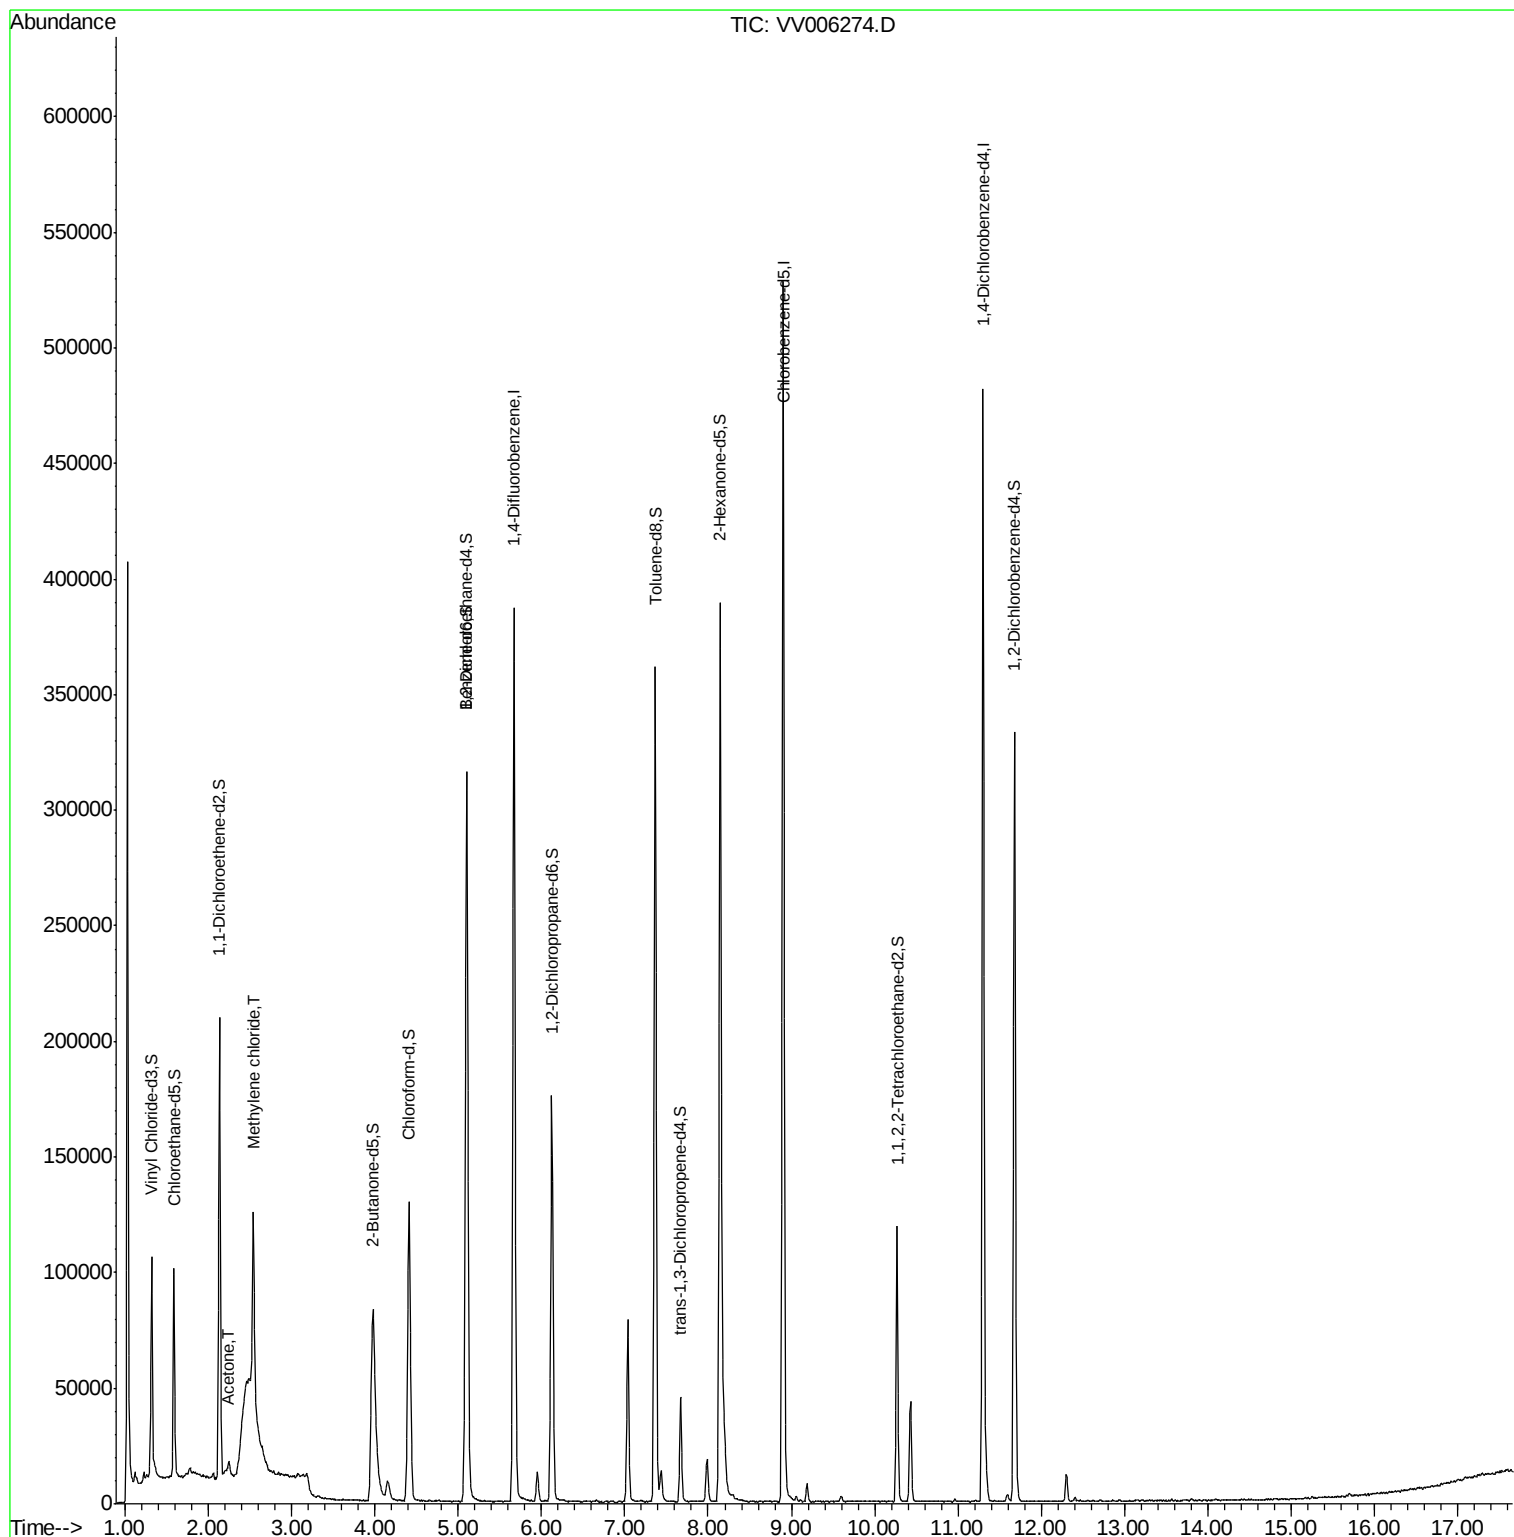

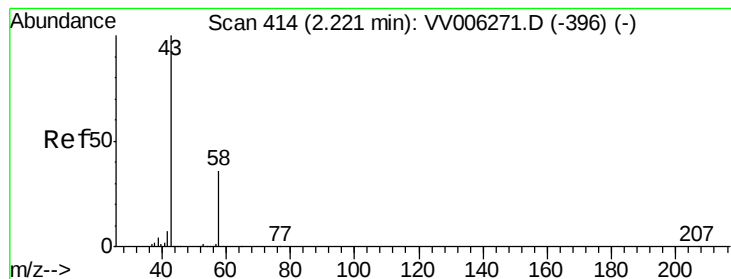

#13

Acetone

Concen: 3.396 ug/L

RT: 2.22 min Scan# 415

Delta R.T. 0.00 min

Lab File: VV006274.D

Acq: 15 Jun 2018 11:32

Instrument :

MSVOA_V

ClientSampleId :





BEXW2

Tgt Ion: 43 Resp: 7286

Ion Ratio Lower Upper

43 100

58 45.6 0.0 67.4

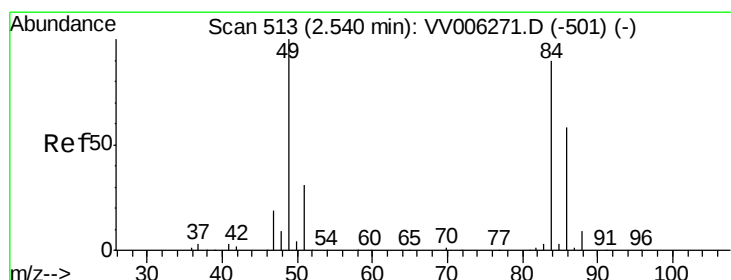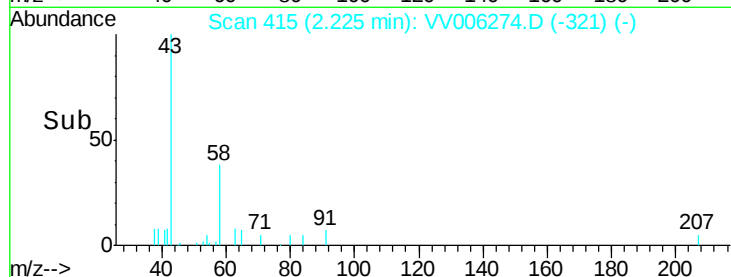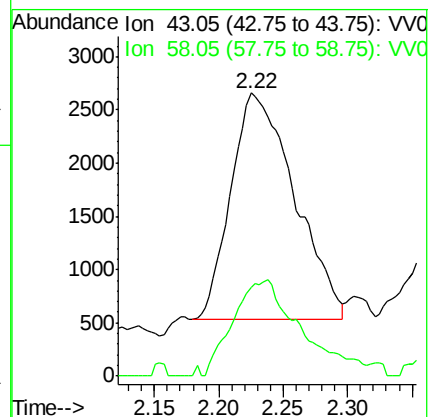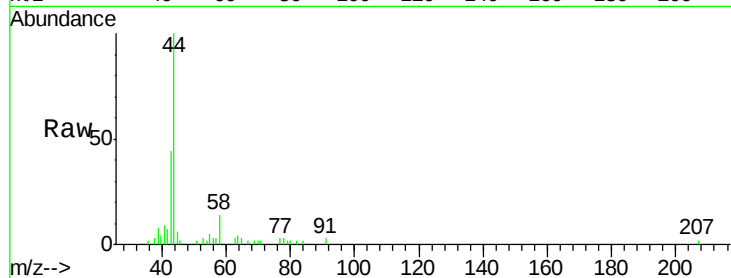

#16

Methylene chloride

Concen: 1.593 ug/L

RT: 2.54 min Scan# 513

Delta R.T. 0.00 min

Lab File: VV006274.D

Acq: 15 Jun 2018 11:32

Tgt Ion: 84 Resp: 34466

Ion Ratio Lower Upper

84 100

86 64.7 44.2 82.0

49 110.0 78.8 146.4

