

Data File : VV006278.D
Acq On : 15 Jun 2018 13:20
Operator : SY/MD
Sample : J3507-19
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWD1

Quant Time: Jun 16 00:16:44 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 15 23:47:49 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	298189	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	268101	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	121675	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	55715	3.42	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.40%
7) Chloroethane-d5	1.58	69	58035	4.45	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.00%
11) 1,1-Dichloroethene-d2	2.13	63	84703	2.68	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	53.60%#
20) 2-Butanone-d5	3.95	46	223691	64.69	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	129.38%
24) Chloroform-d	4.41	84	137714	4.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.40%
26) 1,2-Dichloroethane-d4	5.09	65	73805	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
32) Benzene-d6	5.11	84	265893	4.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.60%
36) 1,2-Dichloropropane-d6	6.12	67	86553	4.47	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.40%
41) Toluene-d8	7.37	98	229571	3.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.80%
43) trans-1,3-Dichloropropene-	7.67	79	29243	3.37	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	67.40%
46) 2-Hexanone-d5	8.14	63	188161	50.28	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.56%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	69735	4.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	99192	4.70	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.00%


Target Compounds					Qvalue
13) Acetone	2.20	43	12081	6.447 ug/L	90
14) Carbon disulfide	2.32	76	23594	0.412 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV006278.D
Acq On : 15 Jun 2018 13:20
Operator : SY/MD
Sample : J3507-19
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWD1

Quant Time: Jun 16 00:16:44 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 15 23:47:49 2018
Response via : Initial Calibration

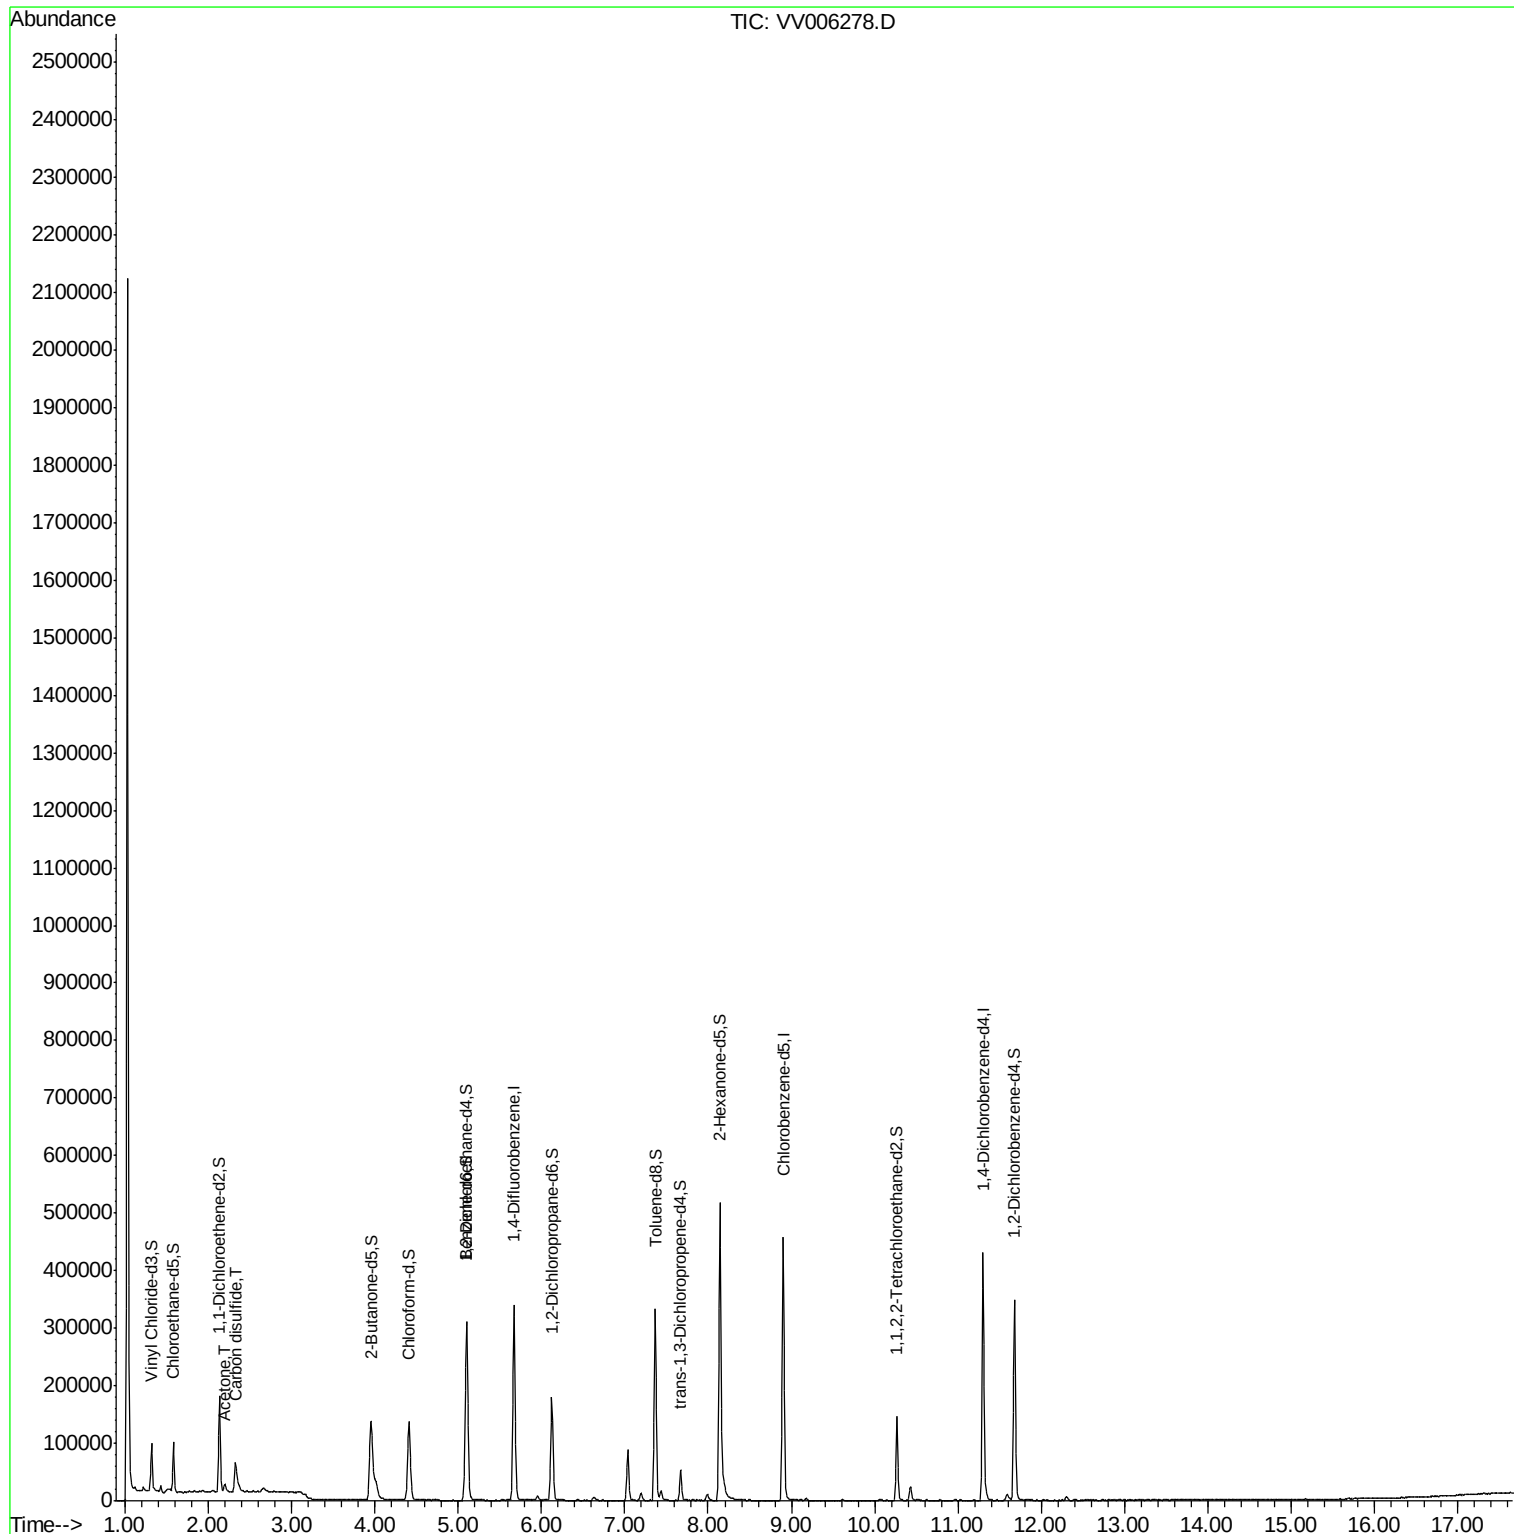

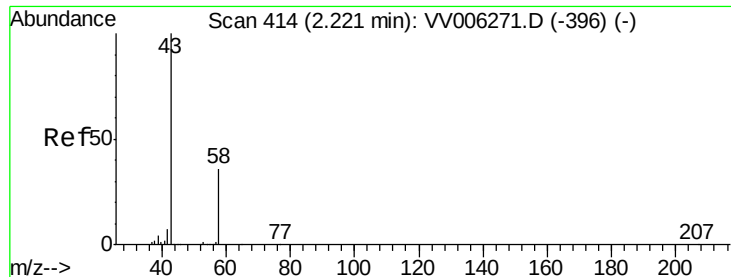

#13

Acetone

Concen: 6.447 ug/L

RT: 2.20 min Scan# 407

Delta R.T. -0.02 min

Lab File: VV006278.D

Acq: 15 Jun 2018 13:20

Instrument :

MSVOA_V

ClientSampleId :





ESWD1

Tgt Ion: 43 Resp: 12081

Ion Ratio Lower Upper

43 100

58 39.4 0.0 67.4

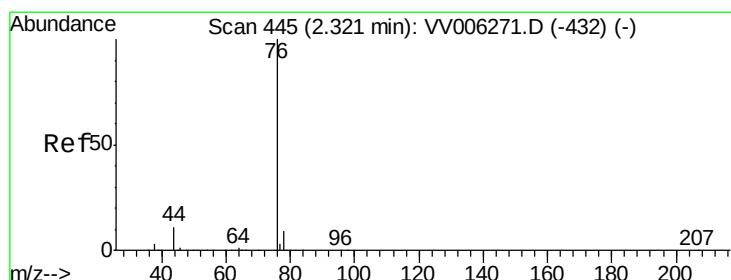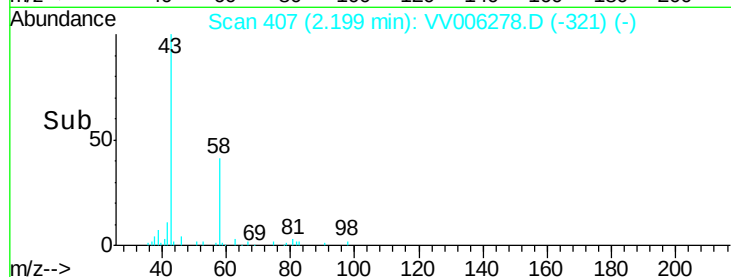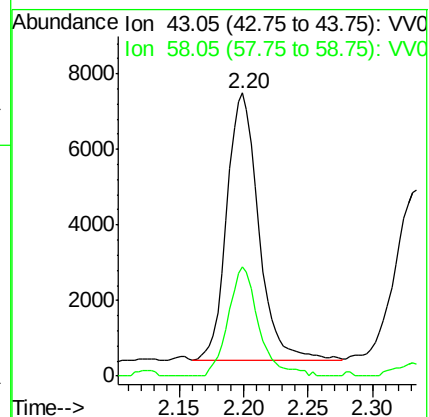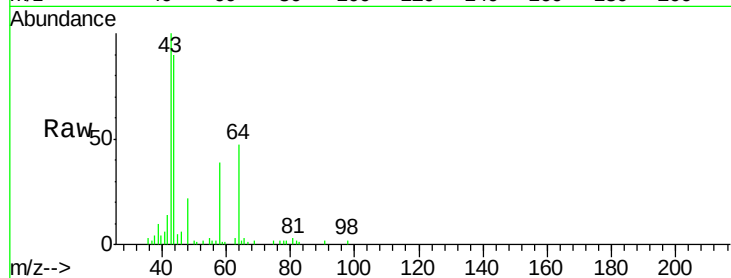

#14

Carbon disulfide

Concen: 0.412 ug/L

RT: 2.32 min Scan# 445

Delta R.T. 0.00 min

Lab File: VV006278.D

Acq: 15 Jun 2018 13:20

Tgt Ion: 76 Resp: 23594

Ion Ratio Lower Upper

76 100

78 10.4 7.5 11.3

