

Data File : VV006299.D
Acq On : 16 Jun 2018 00:02
Operator : SY/MD
Sample : J3473-10
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KB4

Quant Time: Jun 16 01:11:41 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 16 00:57:31 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	270465	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	241980	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	108846	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	64111	4.34	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.80%
7) Chloroethane-d5	1.59	69	62891	5.32	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.40%
11) 1,1-Dichloroethene-d2	2.13	63	91156	3.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.60%
20) 2-Butanone-d5	3.97	46	204669	65.25	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	130.50%#
24) Chloroform-d	4.41	84	142336	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.60%
26) 1,2-Dichloroethane-d4	5.09	65	73823	5.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.80%
32) Benzene-d6	5.11	84	280020	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.40%
36) 1,2-Dichloropropane-d6	6.13	67	89552	5.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.40%
41) Toluene-d8	7.37	98	242089	4.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.40%
43) trans-1,3-Dichloropropene-	7.67	79	25796	3.30	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	66.00%
46) 2-Hexanone-d5	8.14	63	156247	46.26	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.52%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	65158	5.15	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	98391	5.21	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.20%


Target Compounds					Qvalue
13) Acetone	2.22	43	9255	5.445 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV006299.D
Acq On : 16 Jun 2018 00:02
Operator : SY/MD
Sample : J3473-10
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KB4

Quant Time: Jun 16 01:11:41 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 16 00:57:31 2018
Response via : Initial Calibration

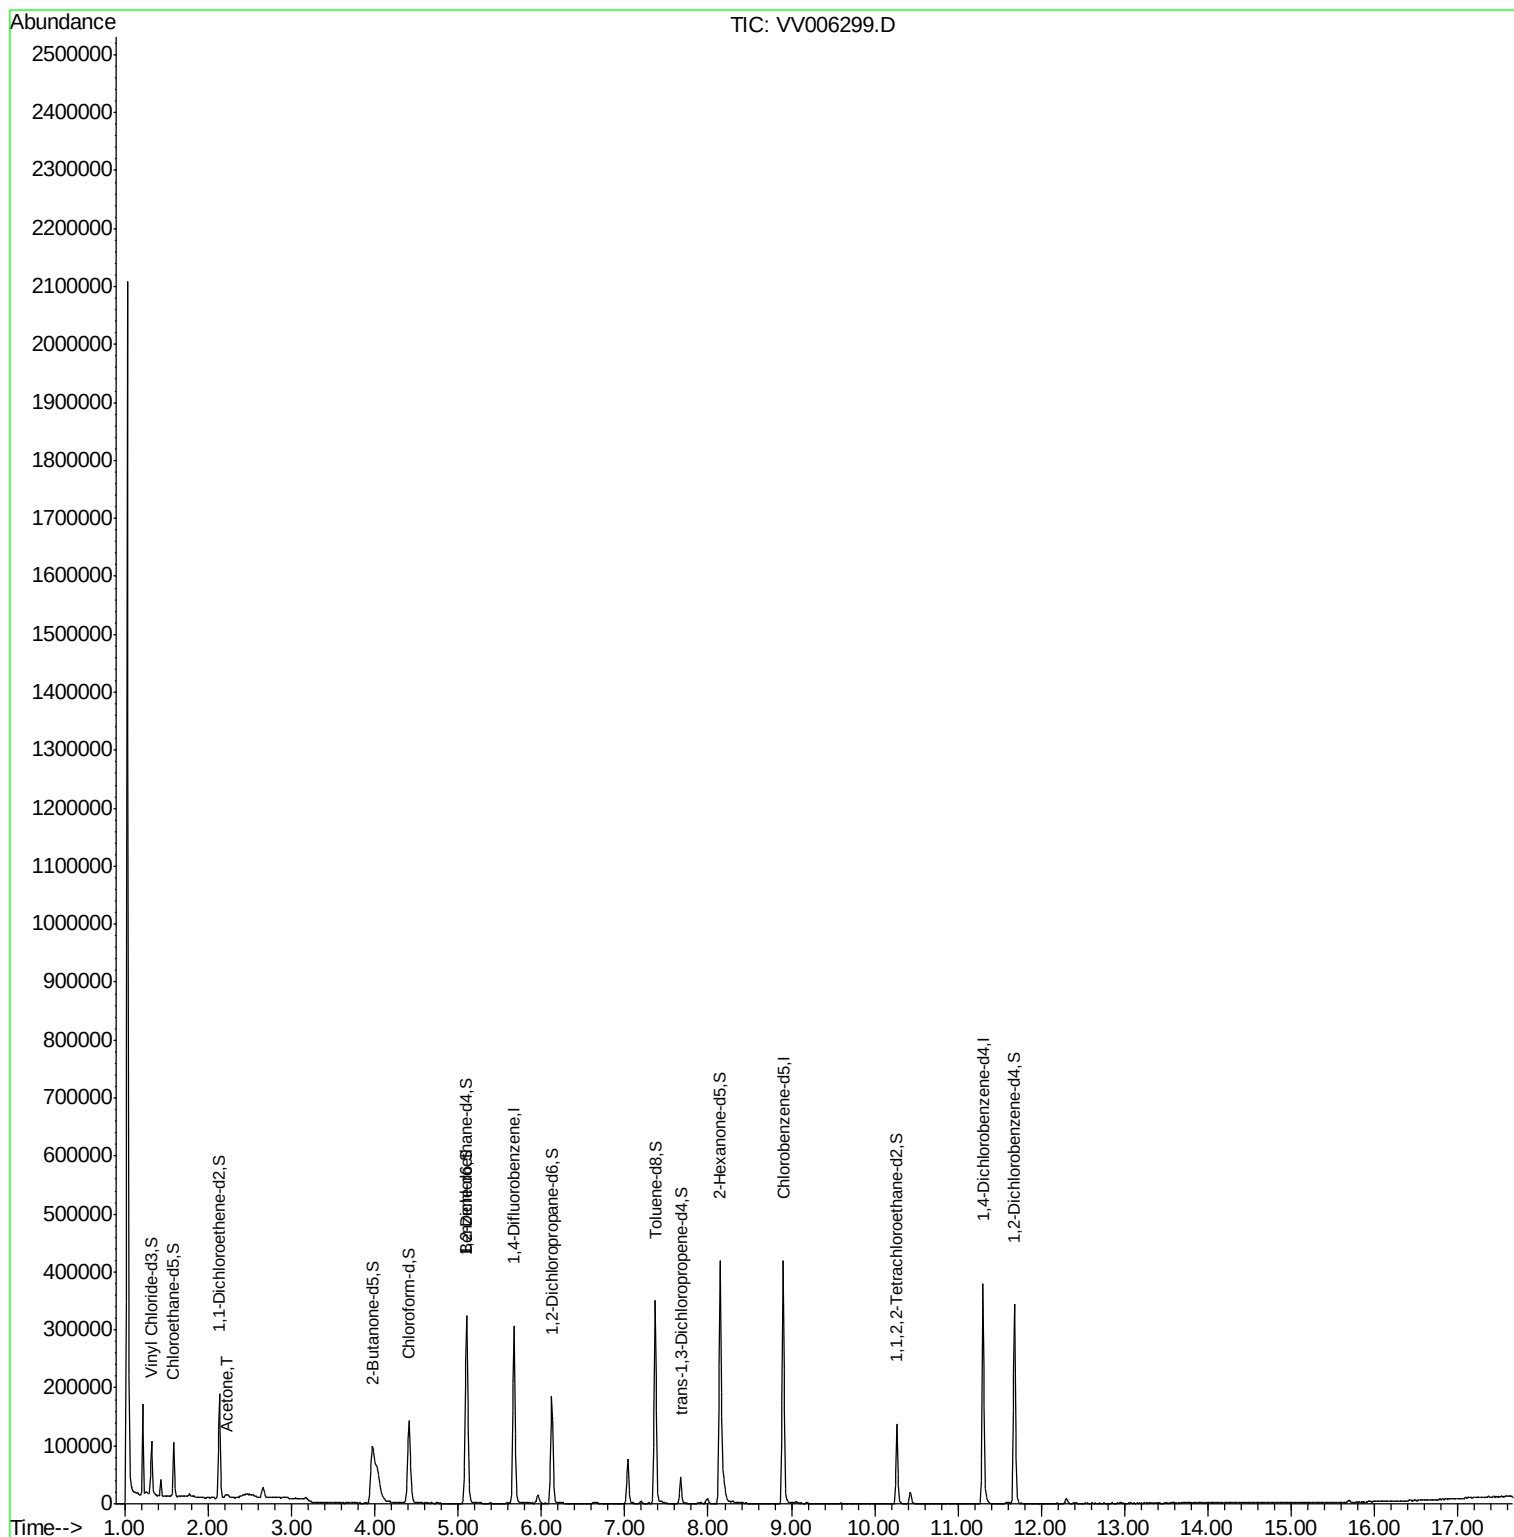

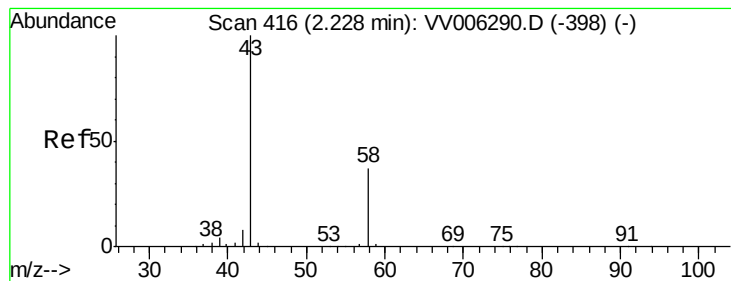

#13
 Acetone
 Concen: 5.445 ug/L
 RT: 2.22 min Scan# 413
 Delta R.T. -0.01 min
 Lab File: VV006299.D
 Acq: 16 Jun 2018 00:02

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KB4

Tgt Ion: 43 Resp: 9255
 Ion Ratio Lower Upper
 43 100
 58 34.2 0.0 67.4

