

Data File : VV006301.D
Acq On : 16 Jun 2018 00:56
Operator : SY/MD
Sample : J3473-12
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KB6

Quant Time: Jun 16 01:26:38 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 16 00:57:31 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	260014	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	234114	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	103846	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	65149	4.59	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.80%
7) Chloroethane-d5	1.58	69	63272	5.56	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.20%
11) 1,1-Dichloroethene-d2	2.13	63	92624	3.36	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.20%
20) 2-Butanone-d5	3.95	46	212598	70.51	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	141.02%#
24) Chloroform-d	4.41	84	142120	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.40%
26) 1,2-Dichloroethane-d4	5.09	65	75765	5.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	114.00%
32) Benzene-d6	5.11	84	286436	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.80%
36) 1,2-Dichloropropane-d6	6.12	67	92674	5.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.60%
41) Toluene-d8	7.37	98	245871	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
43) trans-1,3-Dichloropropene-	7.67	79	26035	3.44	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.80%
46) 2-Hexanone-d5	8.14	63	164347	50.29	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.58%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	65911	5.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	100685	5.59	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.80%


Target Compounds					Qvalue
13) Acetone	2.20	43	13735	8.406 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV006301.D
Acq On : 16 Jun 2018 00:56
Operator : SY/MD
Sample : J3473-12
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KB6

Quant Time: Jun 16 01:26:38 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 16 00:57:31 2018
Response via : Initial Calibration

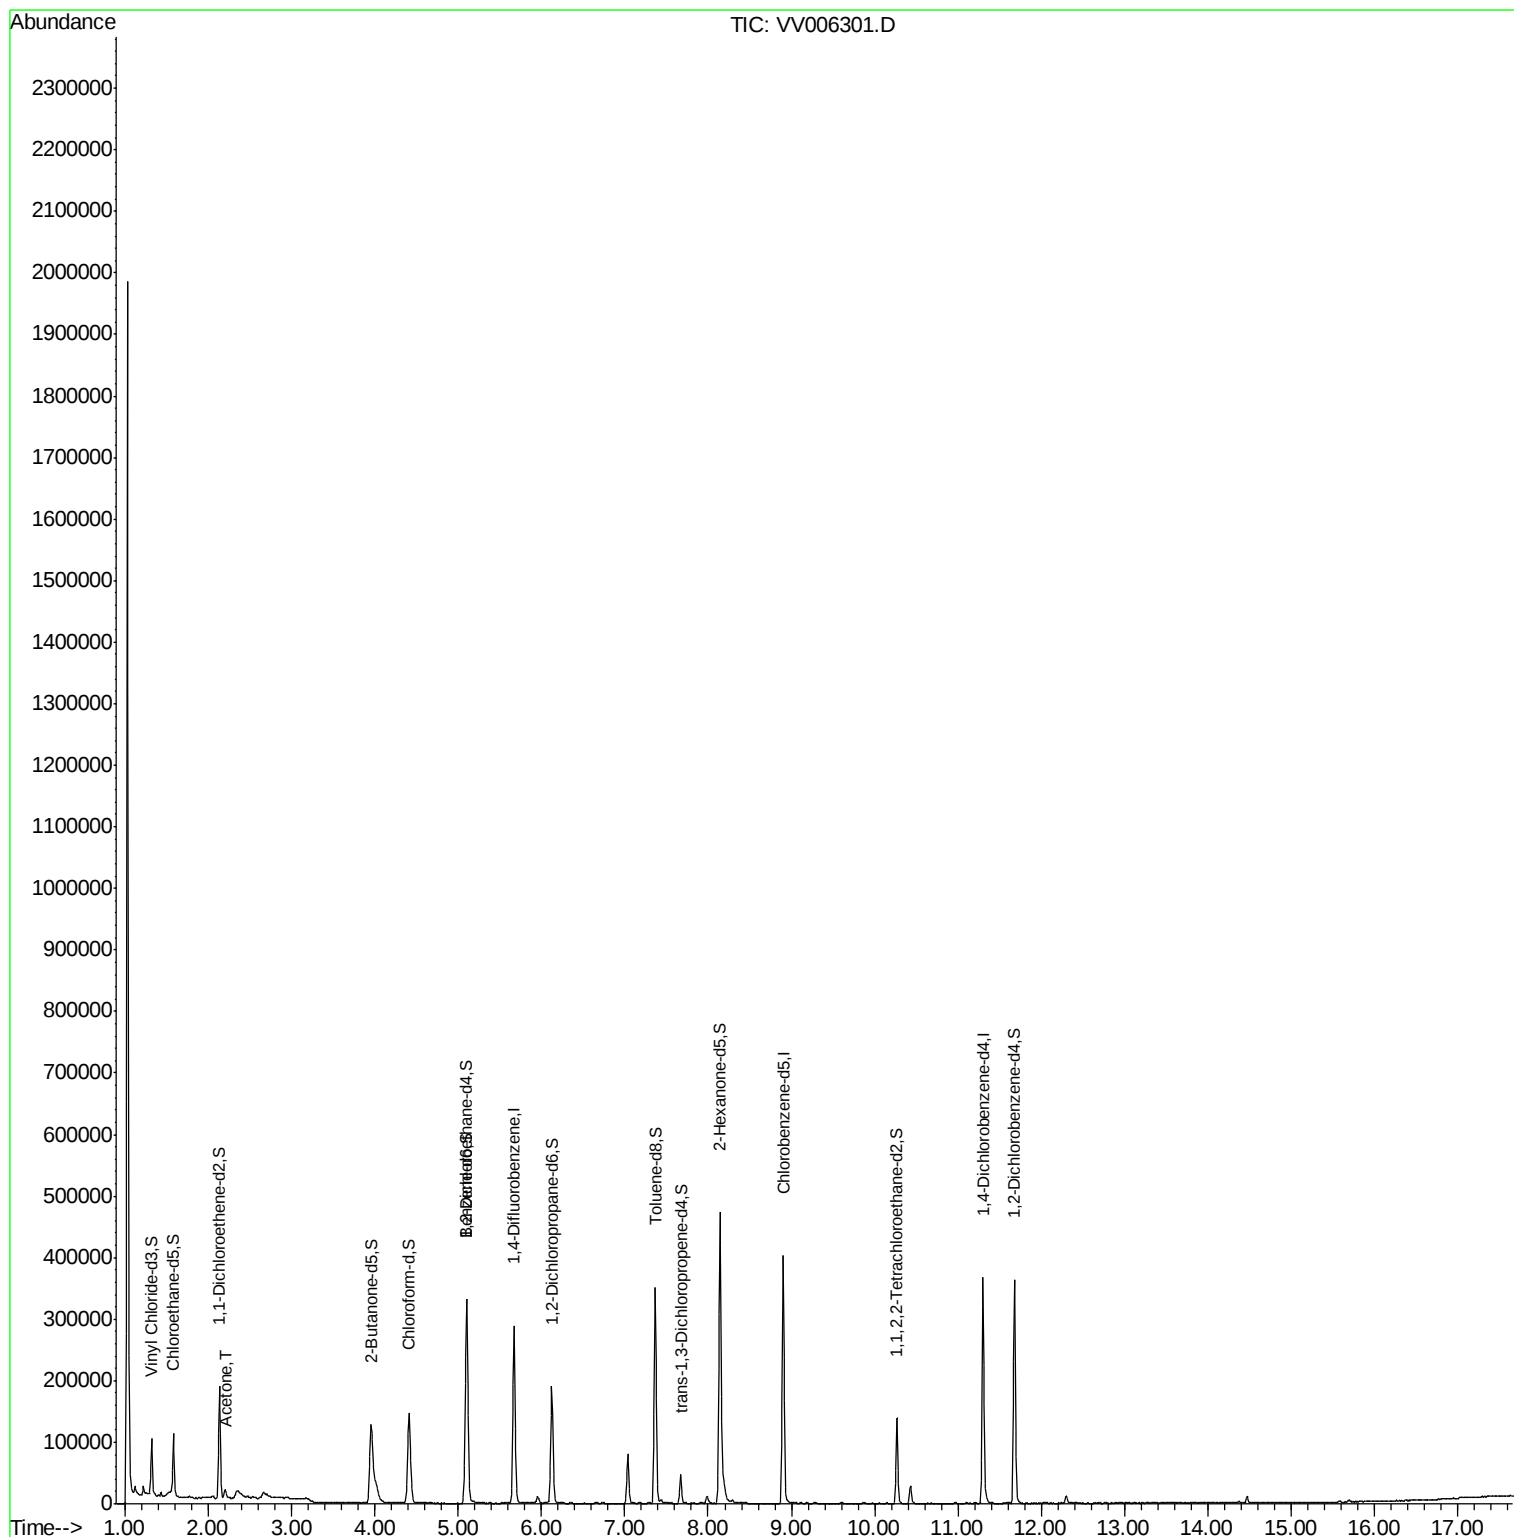

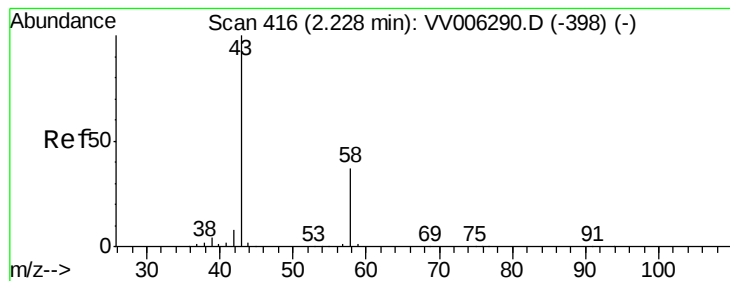

#13

Acetone

Concen: 8.406 ug/L

RT: 2.20 min Scan# 408

Delta R.T. -0.03 min

Lab File: VV006301.D

Acq: 16 Jun 2018 00:56

Instrument :
MSVOA_V
ClientSampleId :
C0KB6

Tgt Ion: 43 Resp: 13735

Ion Ratio Lower Upper

43 100

58 38.0 0.0 67.4

