

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061518\
 Data File : VV006280.D
 Acq On : 15 Jun 2018 14:14
 Operator : SY/MD
 Sample : J3397-04DL 5X
 Misc : 25 mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEXT3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.028	29	43	67	rBV	1524364	1826292	100.00%	15.963%
2	1.321	125	134	160	rVB	126681	159275	8.72%	1.392%
3	1.430	161	168	174	rBV	77320	79338	4.34%	0.693%
4	1.575	206	213	233	rVB	102012	125842	6.89%	1.100%
5	2.131	376	386	398	rBV	243459	345227	18.90%	3.017%
6	2.598	521	531	538	rBV	34116	59770	3.27%	0.522%
7	2.655	538	549	573	rVB	178909	398581	21.82%	3.484%
8	3.958	934	954	959	rBV2	177422	461317	25.26%	4.032%
9	4.408	1077	1094	1117	rVB	148424	356904	19.54%	3.120%
10	5.099	1291	1309	1330	rBV2	371328	892240	48.86%	7.799%
11	5.668	1469	1486	1506	rBV	340959	665399	36.43%	5.816%
12	5.964	1564	1578	1591	rVB5	23592	50984	2.79%	0.446%
13	6.125	1612	1628	1653	rBV	200824	405099	22.18%	3.541%
14	7.035	1899	1911	1929	rBV	109409	191628	10.49%	1.675%
15	7.366	2000	2014	2030	rBV	461425	796501	43.61%	6.962%
16	7.668	2097	2108	2125	rBV	65644	108653	5.95%	0.950%
17	8.138	2237	2254	2300	rBV	472026	923965	50.59%	8.076%
18	8.903	2477	2492	2495	rBV	497224	743394	40.71%	6.498%
19	8.928	2495	2500	2527	rVB	747346	1211798	66.35%	10.592%
20	10.269	2902	2917	2934	rBV	147887	233599	12.79%	2.042%
21	11.301	3225	3238	3266	rVB	432166	734330	40.21%	6.418%
22	11.678	3343	3355	3380	rBV	405085	670787	36.73%	5.863%


Sum of corrected areas: 11440923

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061518\
Data File : VV006280.D
Acq On : 15 Jun 2018 14:14
Operator : SY/MD
Sample : J3397-04DL 5X
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEXT3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

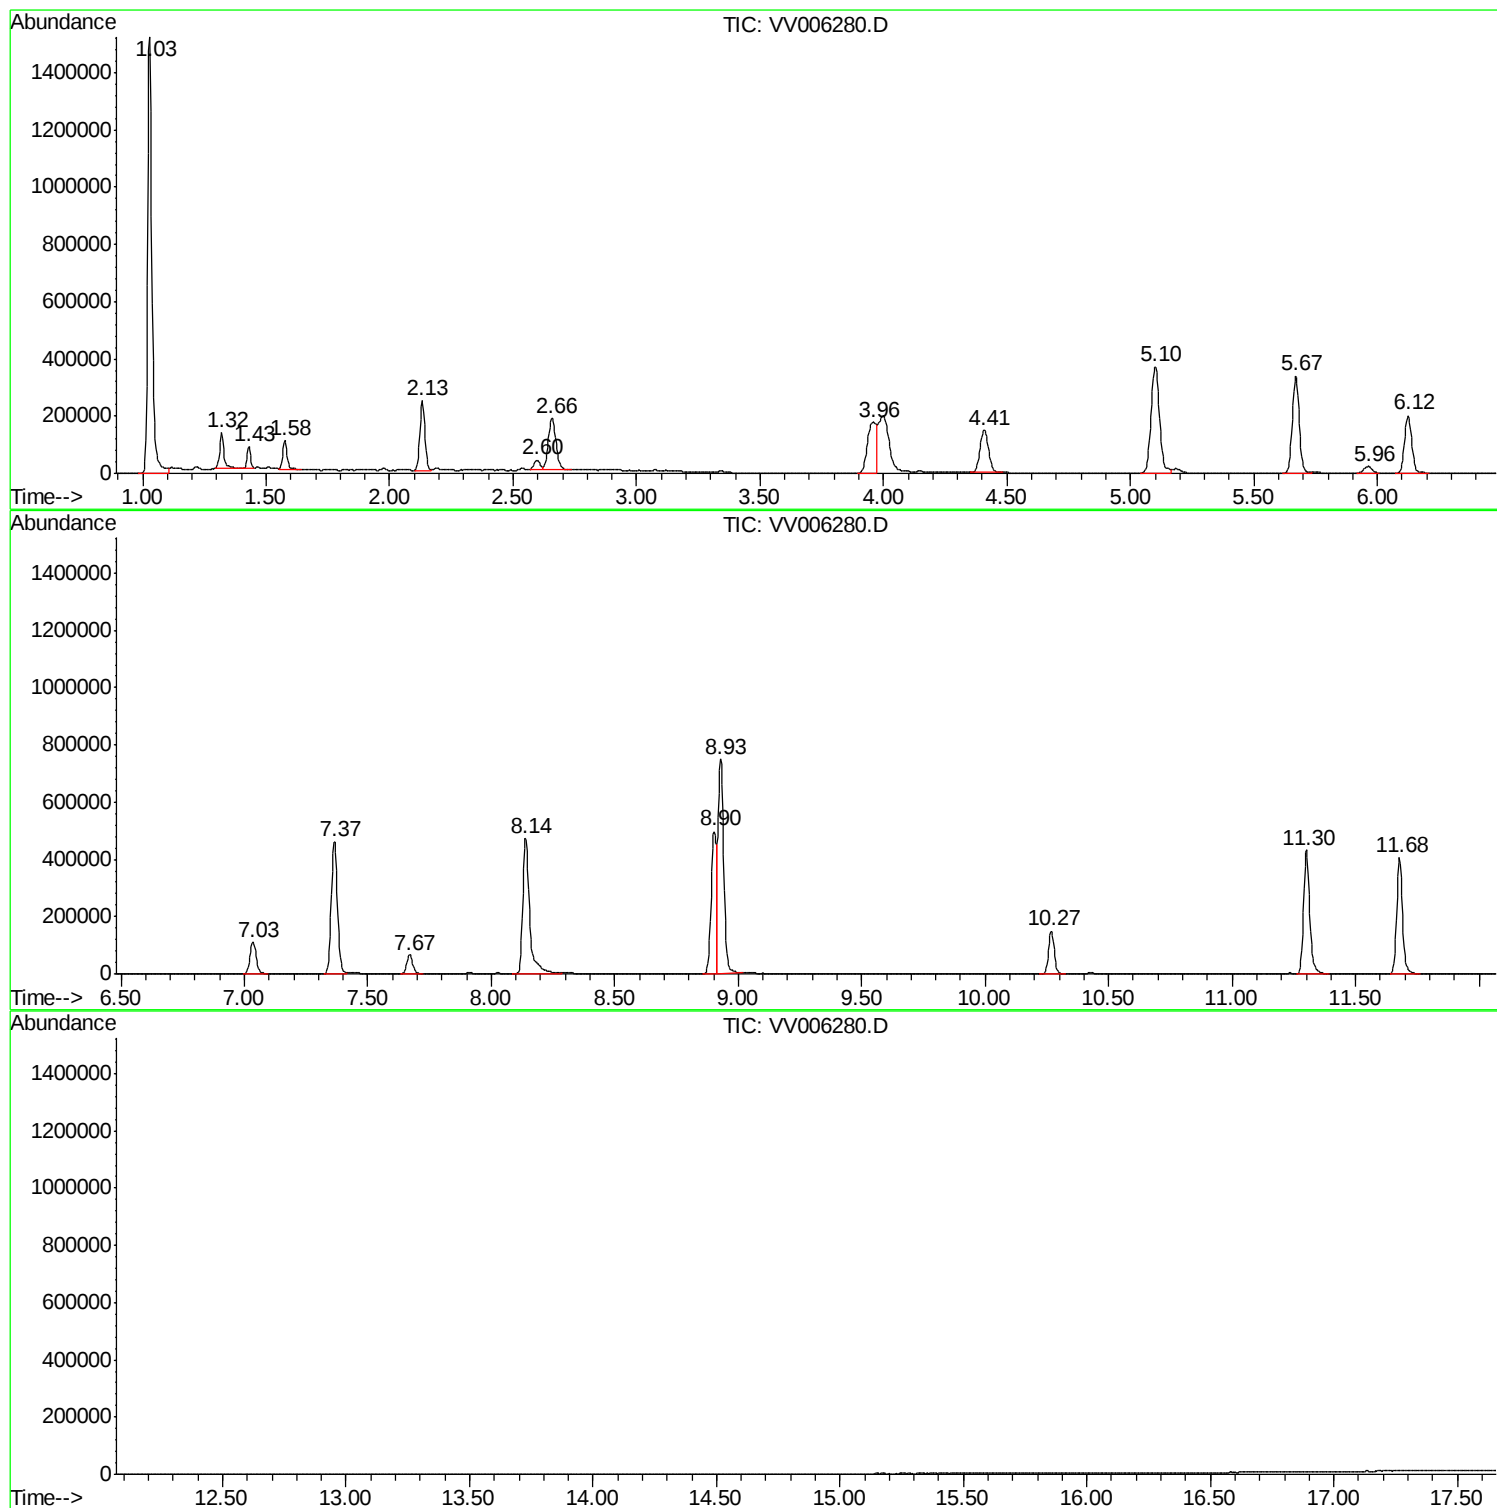

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061518\
 Data File : VV006280.D
 Acq On : 15 Jun 2018 14:14
 Operator : SY/MD
 Sample : J3397-04DL 5X
 Misc : 25 mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEXT3DL










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
 TIC Integration Parameters: LSCINT.P

 Peak Number 2 Trimethylsilyl fluoride Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.43	0.60 ug/L	79338	1,4-Difluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Trimethylsilyl fluoride	92	C3H9FSi	000420-56-4	91
2		Trimethylsilyl fluoride	92	C3H9FSi	000420-56-4	91
3		Propane, 1,2-dichloro-2-methyl-	126	C4H8Cl2	000594-37-6	38
4		Trimethylphosphine oxide	92	C3H9OP	000676-96-0	4
5		2-Propanone, 1,1,3-trichloro-	160	C3H3Cl3O	000921-03-9	2

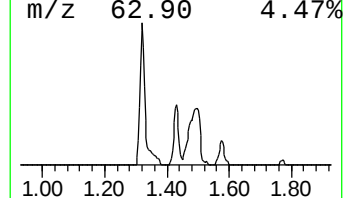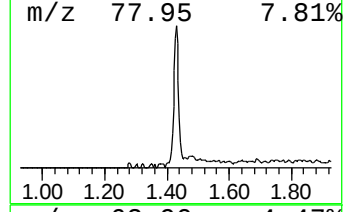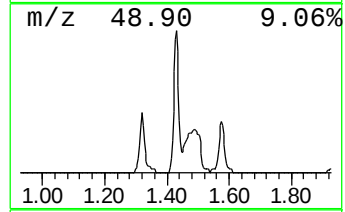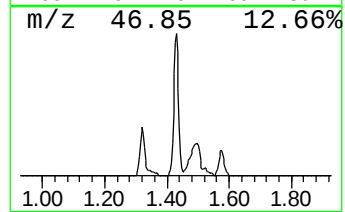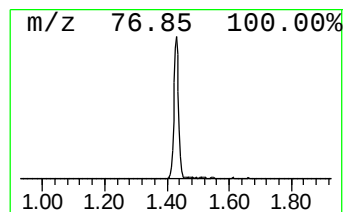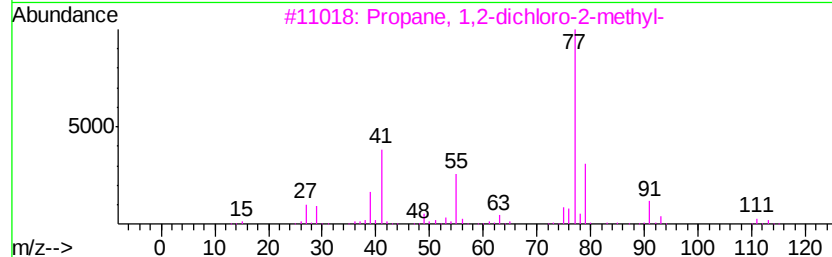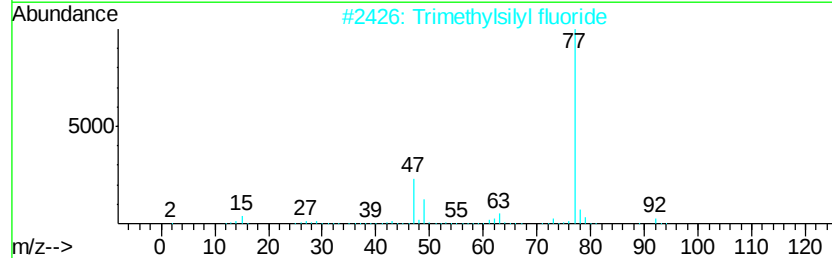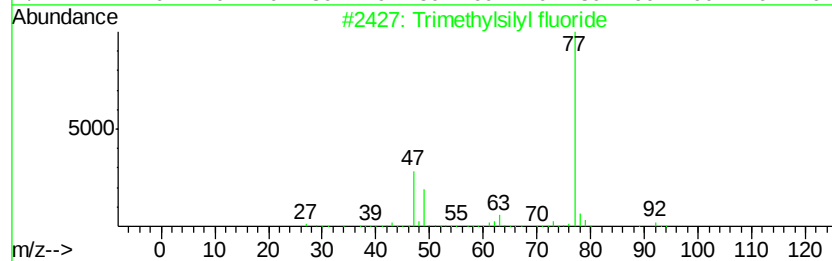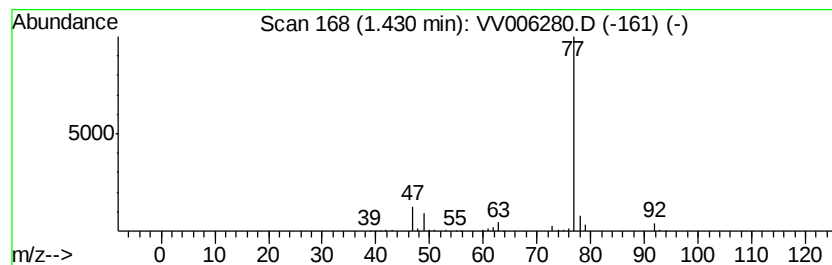

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061518\
Data File : VV006280.D
Acq On : 15 Jun 2018 14:14
Operator : SY/MD
Sample : J3397-04DL 5X
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEXT3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trimethylsilyl fl...	1.43	0.6	ug/L	79338	1	5.67	665399	5.0