

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061518\
 Data File : VV006281.D
 Acq On : 15 Jun 2018 14:41
 Operator : SY/MD
 Sample : J3397-03DL 50X
 Misc : 25 mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEXT2DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.029	31	43	66	rBV	1232281	1419158	32.35%	9.826%
2	1.321	125	134	156	rVB	121596	148839	3.39%	1.030%
3	1.582	208	215	231	rVB	108259	136409	3.11%	0.944%
4	2.135	377	387	399	rBV	245485	342286	7.80%	2.370%
5	3.955	936	953	965	rBV	116340	321915	7.34%	2.229%
6	4.411	1076	1095	1121	rBV	161671	389643	8.88%	2.698%
7	5.102	1291	1310	1315	rBV2	376153	788681	17.98%	5.460%
8	5.154	1316	1326	1352	rVB	2077437	4387545	100.00%	30.377%
9	5.672	1471	1487	1513	rBV	329580	646449	14.73%	4.476%
10	6.125	1612	1628	1650	rBV	202483	405189	9.23%	2.805%
11	7.035	1898	1911	1929	rBV	104166	186093	4.24%	1.288%
12	7.366	2000	2014	2029	rBV	453238	787858	17.96%	5.455%
13	7.668	2097	2108	2121	rBV	62549	105420	2.40%	0.730%
14	8.141	2242	2255	2291	rBV	429320	830972	18.94%	5.753%
15	8.903	2478	2492	2495	rBV	473123	709501	16.17%	4.912%
16	8.929	2496	2500	2529	rVV	682091	1036965	23.63%	7.179%
17	9.060	2530	2541	2556	rVB	129315	202427	4.61%	1.402%
18	9.189	2570	2581	2595	rBV	39515	61832	1.41%	0.428%
19	10.269	2905	2917	2937	rBV	135238	211131	4.81%	1.462%
20	11.302	3226	3238	3259	rBV	407791	674782	15.38%	4.672%
21	11.678	3343	3355	3382	rBV	405057	650379	14.82%	4.503%


Sum of corrected areas: 14443474

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061518\
Data File : VV006281.D
Acq On : 15 Jun 2018 14:41
Operator : SY/MD
Sample : J3397-03DL 50X
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEXT2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

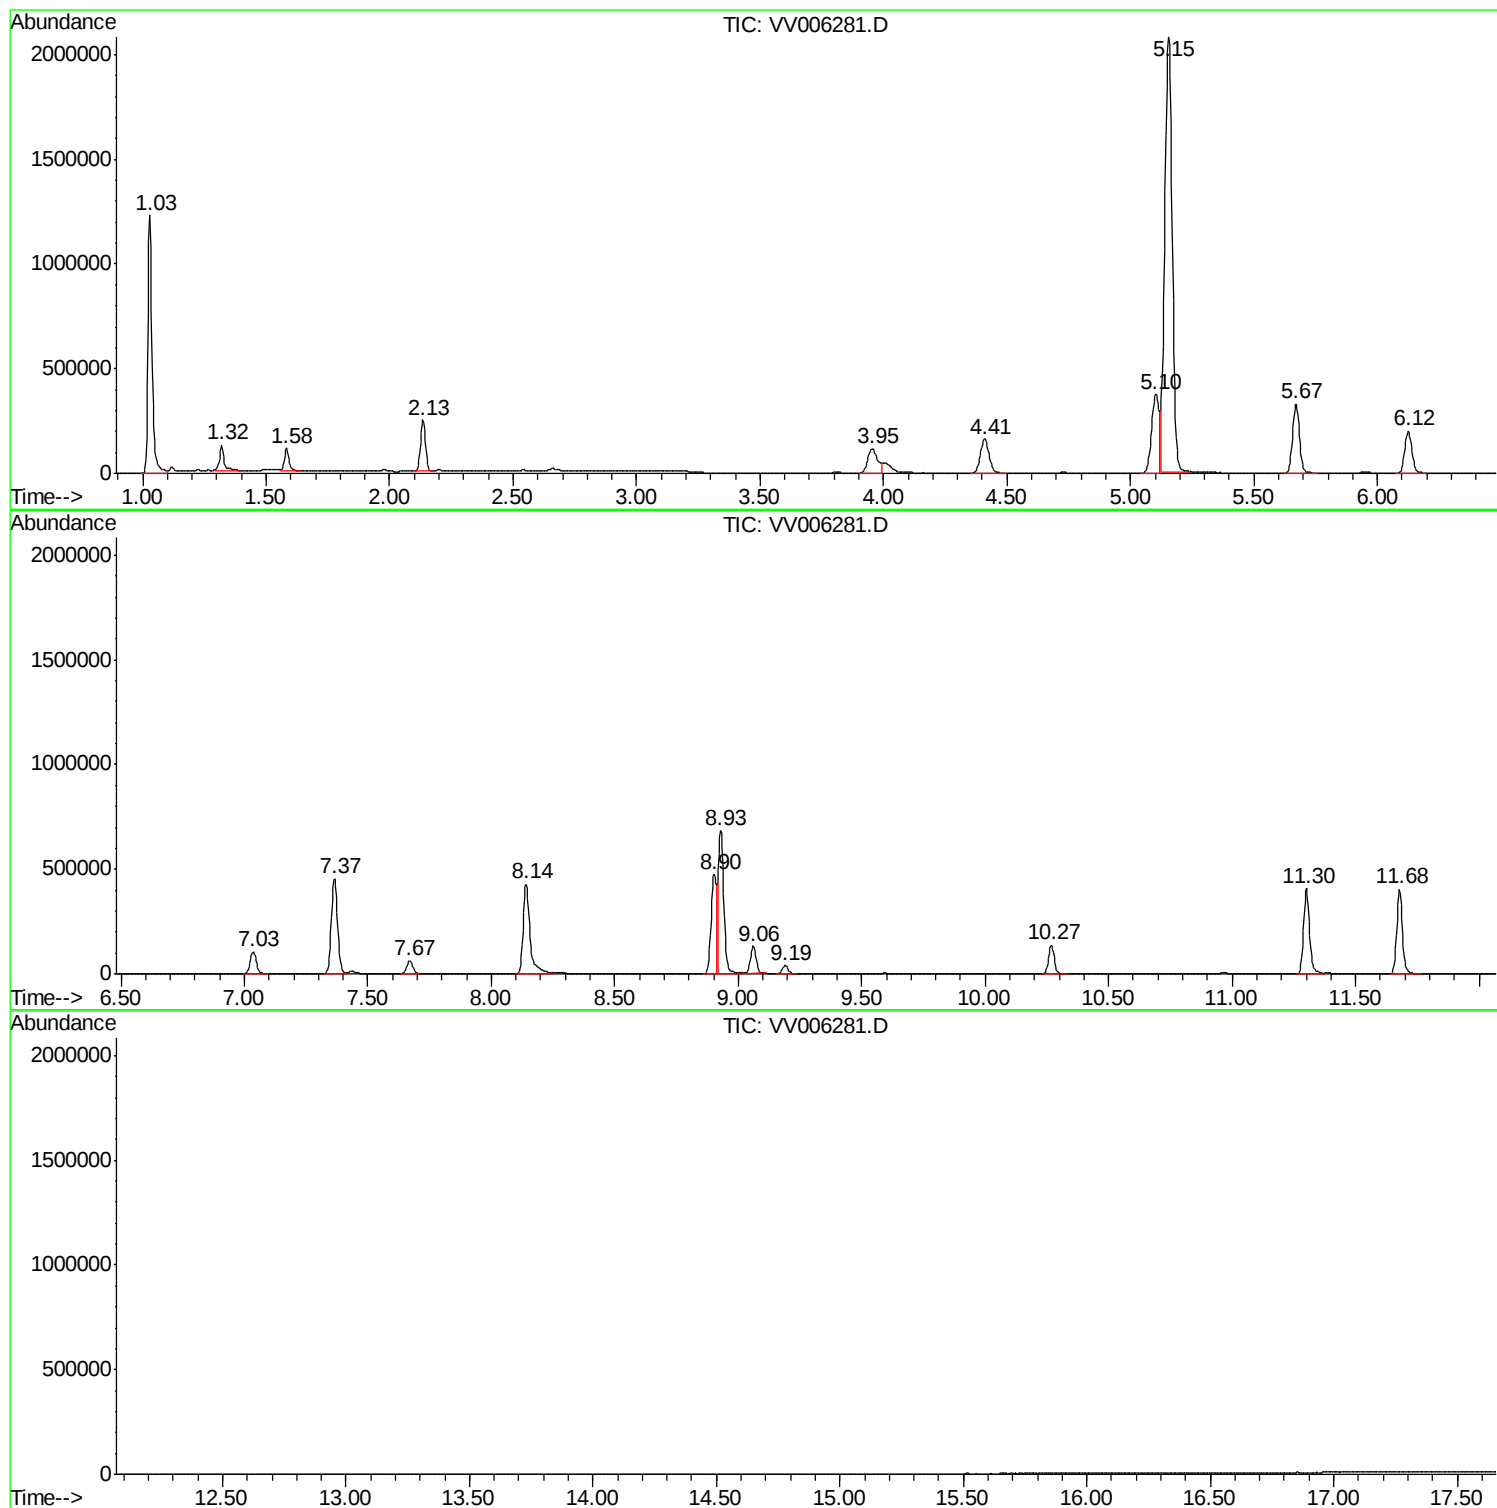

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061518\
Data File : VV006281.D
Acq On : 15 Jun 2018 14:41
Operator : SY/MD
Sample : J3397-03DL 50X
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEXT2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061518\
Data File : VV006281.D
Acq On : 15 Jun 2018 14:41
Operator : SY/MD
Sample : J3397-03DL 50X
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEXT2DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc