


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061518\
Data File : VV006270.D
Acq On : 15 Jun 2018 08:58
Operator : SY/MD
Sample : BFB72
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB72

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Jun 18 03:14:32 2018

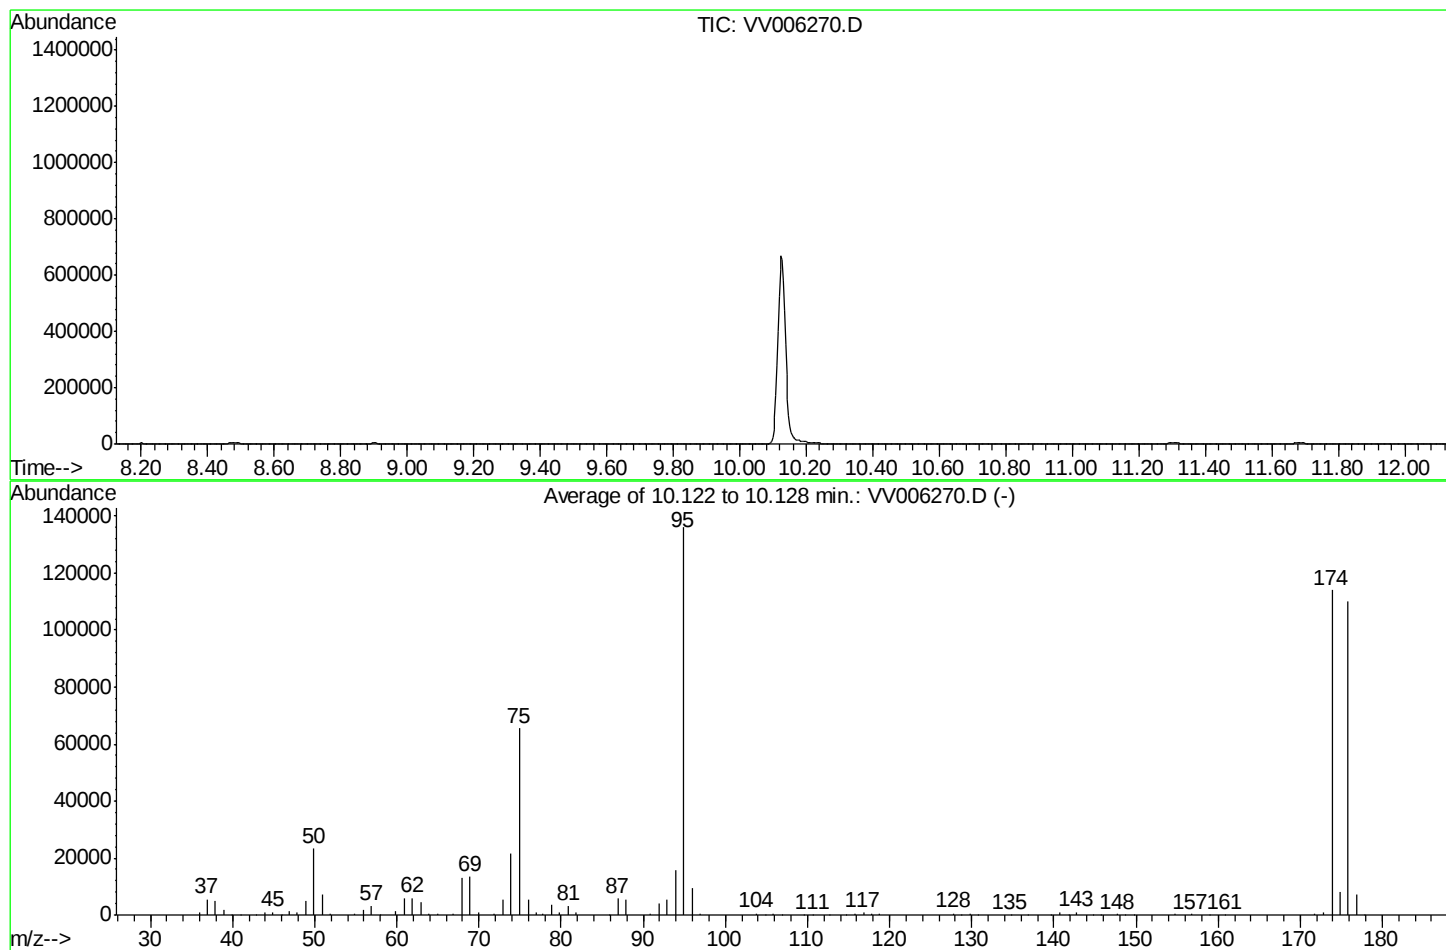

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	23274	PASS
75	95	30	80	48.1	65517	PASS
95	95	100	100	100.0	136085	PASS
96	95	5	9	7.0	9481	PASS
173	174	0.00	2	0.7	749	PASS
174	95	50	120	83.8	114021	PASS
175	174	5	9	7.2	8251	PASS
176	174	95	101	96.5	110085	PASS
177	176	5	9	6.6	7280	PASS

Scan 2858 (10.080 min): VV006270.D
BFB72

m/z	Abundance
39.80	124.0
42.90	115.0
43.90	612.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
35.90	790.0
36.90	5259.0
37.90	4684.0
38.90	1883.0
39.90	199.0
43.00	149.0
43.90	1355.0
44.90	881.0
46.90	1233.0
47.80	693.0
48.90	4579.0
49.90	22584.0
50.90	7061.0
51.90	365.0
54.90	356.0
55.90	1850.0
56.90	3118.0
57.90	193.0
59.90	1219.0
60.90	5607.0
61.90	5736.0
62.90	4251.0
64.00	505.0
65.00	230.0
66.90	419.0
67.90	12538.0
68.90	12702.0
69.90	1079.0
71.90	610.0
72.90	5378.0
73.90	20824.0
74.90	63384.0
76.00	5211.0
77.00	825.0
77.70	522.0
78.80	3308.0
79.80	1028.0
80.90	3237.0
81.80	654.0
85.90	164.0
86.90	5603.0
87.90	5608.0
90.80	413.0
91.90	3791.0
92.90	5373.0
93.90	15127.0
94.90	131200.0
96.00	9314.0
96.90	216.0
103.80	539.0
104.80	174.0
105.70	441.0
106.90	116.0
110.70	117.0
114.70	140.0
115.80	398.0
116.80	780.0
117.80	452.0
118.80	571.0
127.80	401.0
128.70	228.0
129.80	407.0
130.80	204.0
134.80	196.0
136.90	175.0
140.80	884.0
141.80	134.0
142.80	1061.0
144.80	104.0
145.70	244.0
147.80	325.0
149.80	115.0
154.70	225.0
156.80	286.0
160.80	177.0
171.80	365.0
172.90	696.0
173.90	107816.0
174.90	7888.0
175.80	103376.0
176.90	6902.0
177.80	195.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
35.90	882.0
36.90	5622.0
37.90	4919.0
38.90	1977.0
39.80	189.0
42.90	129.0
43.90	1368.0
44.90	1035.0
45.90	118.0
46.90	1260.0
47.90	796.0
48.90	4941.0
49.90	24056.0
50.90	7198.0
51.90	356.0
54.80	380.0
55.90	1946.0
56.90	3320.0
58.00	200.0
59.90	1223.0
60.90	6028.0
61.90	6070.0
62.90	4750.0
64.00	529.0
64.90	257.0
66.90	444.0
67.90	13379.0
68.90	13745.0
69.90	1206.0
71.90	714.0
72.90	5702.0
73.90	22120.0
74.90	67456.0
76.00	5587.0
76.90	844.0
77.80	567.0
78.90	3512.0
79.90	1077.0
80.90	3404.0
81.80	752.0
85.90	170.0
86.90	5933.0
87.90	5702.0
90.80	482.0
91.90	4073.0
92.90	5774.0
93.90	16144.0
94.90	140288.0
96.00	9791.0
96.90	240.0
103.80	578.0
104.80	206.0
105.80	489.0
106.90	140.0
112.70	111.0
114.70	127.0
115.80	459.0
116.90	802.0
117.80	484.0
118.80	592.0
127.80	499.0
128.70	214.0
129.80	461.0
130.80	223.0
134.80	220.0
136.80	191.0
139.70	115.0
140.80	937.0
141.80	152.0
142.80	1123.0
144.90	112.0
145.70	245.0
147.70	317.0
148.70	111.0
149.80	130.0
154.70	283.0
156.80	317.0
160.90	188.0
171.80	386.0
172.90	756.0
173.80	117744.0
174.90	8549.0
175.80	113400.0
176.90	7517.0
177.80	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
35.90	922.0
36.90	5396.0
37.90	4676.0
38.90	1892.0
39.80	165.0
41.00	114.0
42.90	123.0
43.90	1302.0
44.90	1032.0
45.90	145.0
46.90	1340.0
47.90	785.0
48.90	4990.0
49.90	23184.0
51.00	6783.0
51.90	314.0
54.80	365.0
55.90	1776.0
56.90	3230.0
58.00	162.0
59.90	1138.0
60.90	5845.0
61.90	5872.0
62.90	4622.0
63.90	501.0
64.90	248.0
66.90	405.0
67.90	13004.0
68.90	13423.0
69.90	1140.0
71.90	706.0
72.90	5783.0
73.90	21464.0
74.90	65712.0
76.00	5506.0
76.90	845.0
77.80	567.0
78.80	3416.0
79.90	1017.0
80.90	3299.0
81.80	801.0
85.90	161.0
86.90	5600.0
87.90	5394.0
90.80	520.0
91.90	3883.0
92.90	5573.0
93.90	15552.0
94.90	136768.0
96.00	9340.0
96.90	287.0
103.80	584.0
104.80	208.0
105.80	463.0
106.90	144.0
109.60	108.0
112.70	149.0
114.70	109.0
115.80	467.0
116.90	741.0
117.80	494.0
118.80	559.0
127.80	559.0
128.70	192.0
129.80	501.0
130.80	227.0
134.80	207.0
136.90	201.0
139.70	127.0
140.80	930.0
141.80	161.0
142.80	1140.0
144.90	120.0
145.70	209.0
147.70	283.0
148.70	103.0
149.80	153.0
154.80	325.0
156.70	283.0
158.90	104.0
160.90	149.0
171.80	359.0
172.90	797.0
173.80	116504.0
174.90	8317.0
175.80	113480.0
176.90	7423.0
177.80	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72