


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016926.D
 Acq On : 15 Jun 2020 10:49
 Operator : SY/MD
 Sample : VV0615WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 16 05:48:34 2020
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 16 05:46:50 2020
 Response via : Initial Calibration

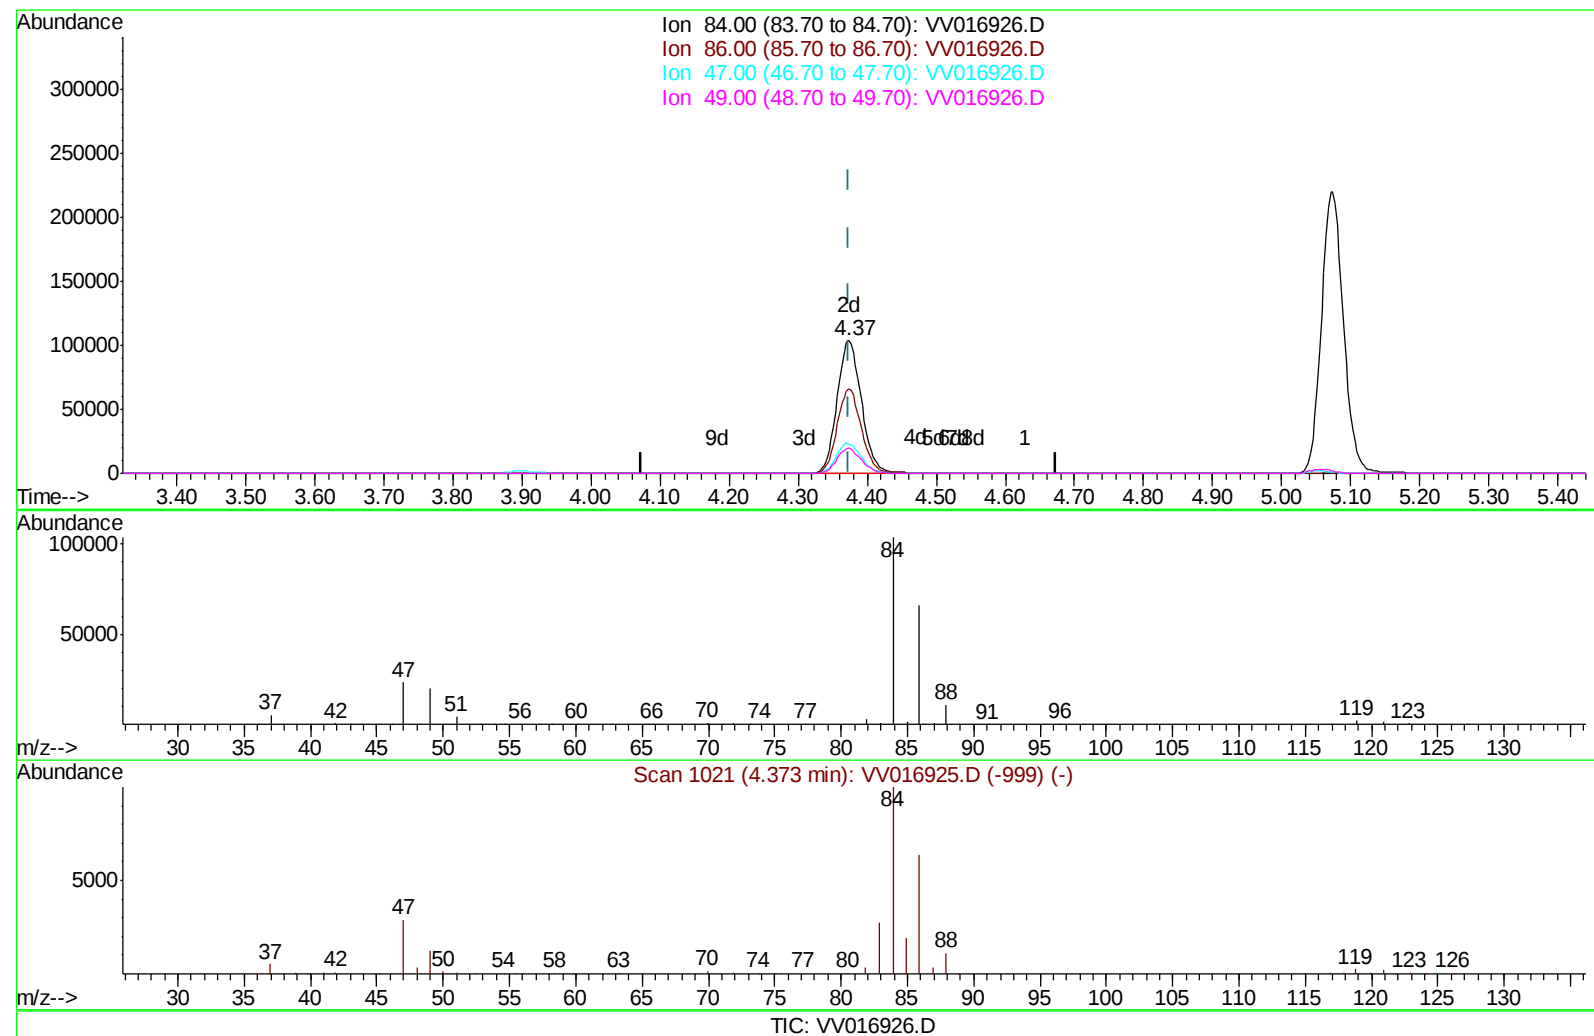

TIC: VV016926.D

(24) Chloroform-d (S)

4.373min (-0.000) 49.78ug/L m

response 251857

Ion	Exp%	Act%
84.00	100	100
86.00	62.80	0.06#
47.00	44.50	0.06#
49.00	27.40	0.04#