

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016926.D
 Acq On : 15 Jun 2020 10:49
 Operator : SY/MD
 Sample : VV0615WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK87

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	192656	190890	12.52%	1.697%
2	1.573	144	150	163	rVB	129429	153061	10.04%	1.360%
3	2.119	311	320	340	rVB	299625	447298	29.33%	3.976%
4	2.354	391	393	398	rBV6	1844	1364	0.09%	0.012%
5	2.415	405	412	414	rBV6	2523	2398	0.16%	0.021%
6	2.473	427	430	434	rBV4	1333	1056	0.07%	0.009%
7	2.618	472	475	477	rBV3	1539	835	0.05%	0.007%
8	2.926	568	571	574	rBV3	2565	2198	0.14%	0.020%
9	3.299	684	687	689	rBV4	1407	832	0.05%	0.007%
10	3.434	726	729	732	rVB5	1176	787	0.05%	0.007%
11	3.479	740	743	746	rBV4	978	675	0.04%	0.006%
12	3.502	746	750	754	rVB6	1283	1343	0.09%	0.012%
13	3.537	759	761	764	rBV3	1065	718	0.05%	0.006%
14	3.560	764	768	772	rBV6	1506	1722	0.11%	0.015%
15	3.595	775	779	780	rBV3	1378	915	0.06%	0.008%
16	3.756	825	829	832	rBV5	1968	1801	0.12%	0.016%
17	3.897	862	873	902	rVV	111812	300489	19.70%	2.671%
18	4.177	958	960	964	rBV4	1978	1418	0.09%	0.013%
19	4.373	1008	1021	1045	rVB	245975	594200	38.96%	5.281%
20	4.608	1090	1094	1095	rBV3	2230	1291	0.08%	0.011%
21	4.769	1141	1144	1149	rBV6	1995	1765	0.12%	0.016%
22	4.823	1157	1161	1162	rBV4	1378	934	0.06%	0.008%
23	5.068	1219	1237	1260	rBV2	588263	1525244	100.00%	13.556%
24	5.640	1402	1415	1434	rBV	429210	850634	55.77%	7.560%
25	5.926	1491	1504	1520	rBV2	35470	76437	5.01%	0.679%
26	6.035	1534	1538	1539	rBV4	1895	1247	0.08%	0.011%
27	6.093	1543	1556	1579	rVB	338976	690608	45.28%	6.138%
28	6.312	1621	1624	1629	rVB6	1285	976	0.06%	0.009%
29	6.344	1630	1634	1636	rBV4	1561	1336	0.09%	0.012%
30	6.492	1678	1680	1682	rBV3	1431	669	0.04%	0.006%
31	6.572	1702	1705	1709	rBV5	2065	1780	0.12%	0.016%
32	6.650	1727	1729	1733	rBV5	1503	1162	0.08%	0.010%
33	6.724	1748	1752	1754	rBV4	2034	1845	0.12%	0.016%
34	6.736	1754	1756	1758	rVV3	1167	674	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016926.D
 Acq On : 15 Jun 2020 10:49
 Operator : SY/MD
 Sample : VV0615WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK87

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.801	1772	1776	1779	rBV5	2591	2078	0.14%	0.018%
36	6.926	1811	1815	1820	rBV7	1661	1668	0.11%	0.015%
37	7.007	1829	1840	1860	rBV2	202022	363602	23.84%	3.232%
38	7.180	1892	1894	1896	rBV4	1784	717	0.05%	0.006%
39	7.334	1929	1942	1959	rBV	713806	1239360	81.26%	11.015%
40	7.566	2010	2014	2016	rBV4	1759	1220	0.08%	0.011%
41	7.640	2026	2037	2058	rBV2	145557	252356	16.55%	2.243%
42	7.920	2119	2124	2127	rBV7	1207	1087	0.07%	0.010%
43	7.939	2127	2130	2132	rBV3	1050	680	0.04%	0.006%
44	8.106	2172	2182	2217	rVV2	327271	641569	42.06%	5.702%
45	8.521	2308	2311	2315	rBV6	1717	1160	0.08%	0.010%
46	8.563	2319	2324	2327	rBV5	1458	1465	0.10%	0.013%
47	8.666	2353	2356	2361	rBV7	1976	1291	0.08%	0.011%
48	8.730	2373	2376	2380	rBV5	1488	1272	0.08%	0.011%
49	8.756	2380	2384	2387	rBV6	1636	1137	0.07%	0.010%
50	8.781	2389	2392	2395	rBV5	1447	1090	0.07%	0.010%
51	8.871	2406	2420	2435	rBV	644109	1036856	67.98%	9.215%
52	9.277	2543	2546	2548	rBV4	1809	1080	0.07%	0.010%
53	9.376	2574	2577	2579	rBV4	1134	880	0.06%	0.008%
54	9.415	2586	2589	2592	rBV4	2163	1625	0.11%	0.014%
55	9.514	2616	2620	2622	rBV3	1880	1224	0.08%	0.011%
56	9.569	2632	2637	2643	rBV10	3213	4546	0.30%	0.040%
57	9.733	2682	2688	2693	rBV10	1574	1915	0.13%	0.017%
58	9.756	2693	2695	2698	rVB4	1417	665	0.04%	0.006%
59	9.891	2735	2737	2740	rBV3	1582	1071	0.07%	0.010%
60	10.016	2773	2776	2778	rBV2	1594	909	0.06%	0.008%
61	10.109	2802	2805	2808	rBV5	1462	1164	0.08%	0.010%
62	10.238	2834	2845	2858	rBV	404034	630005	41.31%	5.599%
63	10.476	2916	2919	2921	rBV3	1567	1109	0.07%	0.010%
64	10.604	2956	2959	2963	rVB4	1517	1095	0.07%	0.010%
65	10.637	2967	2969	2977	rBV9	1433	1677	0.11%	0.015%
66	10.672	2977	2980	2983	rVB4	1923	1087	0.07%	0.010%
67	10.685	2983	2984	2987	rBV3	1226	685	0.04%	0.006%
68	10.778	3009	3013	3014	rBV4	1259	676	0.04%	0.006%
69	10.791	3014	3017	3021	rVB3	1291	1115	0.07%	0.010%
70	10.813	3021	3024	3025	rBV3	2153	1276	0.08%	0.011%
71	10.868	3038	3041	3045	rBV5	3516	2969	0.19%	0.026%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016926.D
 Acq On : 15 Jun 2020 10:49
 Operator : SY/MD
 Sample : VV0615WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK87

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.939	3057	3063	3068	rBV7	2693	3651	0.24%	0.032%
73	10.977	3073	3075	3078	rVV4	1322	772	0.05%	0.007%
74	11.270	3154	3166	3186	rBV	656035	994415	65.20%	8.838%
75	11.646	3271	3283	3302	rBV	748015	1158710	75.97%	10.298%
76	11.846	3341	3345	3347	rBV4	1419	1168	0.08%	0.010%
77	11.910	3363	3365	3368	rBV4	1716	1079	0.07%	0.010%
78	11.968	3380	3383	3384	rBV3	1234	700	0.05%	0.006%
79	12.045	3403	3407	3410	rBV4	1246	1120	0.07%	0.010%
80	12.071	3412	3415	3418	rVB4	1573	992	0.07%	0.009%
81	12.122	3424	3431	3432	rBV5	1812	1986	0.13%	0.018%
82	12.145	3436	3438	3442	rBV3	1704	1138	0.07%	0.010%
83	12.215	3456	3460	3463	rVB4	1405	1100	0.07%	0.010%
84	12.244	3465	3469	3470	rBV3	1524	974	0.06%	0.009%
85	12.286	3478	3482	3486	rVB5	2134	1488	0.10%	0.013%
86	12.437	3527	3529	3535	rBV6	1048	732	0.05%	0.007%
87	12.640	3588	3592	3593	rBV3	1813	1149	0.08%	0.010%
88	12.849	3653	3657	3658	rBV4	1488	981	0.06%	0.009%
89	13.006	3703	3706	3708	rBV3	1220	821	0.05%	0.007%
90	13.019	3708	3710	3712	rVB3	1711	696	0.05%	0.006%
91	13.264	3783	3786	3788	rBV3	1679	1085	0.07%	0.010%
92	13.424	3832	3836	3837	rBV5	1522	1002	0.07%	0.009%
93	13.521	3864	3866	3867	rBV	2536	1161	0.08%	0.010%
94	13.849	3965	3968	3970	rBV4	1270	876	0.06%	0.008%
95	14.006	4014	4017	4020	rBV3	1679	1571	0.10%	0.014%
96	14.344	4120	4122	4127	rBV4	1622	1326	0.09%	0.012%
97	14.379	4132	4133	4136	rVB3	1538	724	0.05%	0.006%
98	14.408	4136	4142	4146	rBV6	1864	2086	0.14%	0.019%
99	15.234	4397	4399	4400	rBV2	1842	868	0.06%	0.008%
100	15.411	4450	4454	4455	rBV3	1278	977	0.06%	0.009%


Sum of corrected areas: 11251331

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061520\
Data File : VV016926.D
Acq On : 15 Jun 2020 10:49
Operator : SY/MD
Sample : VV0615WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK87

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

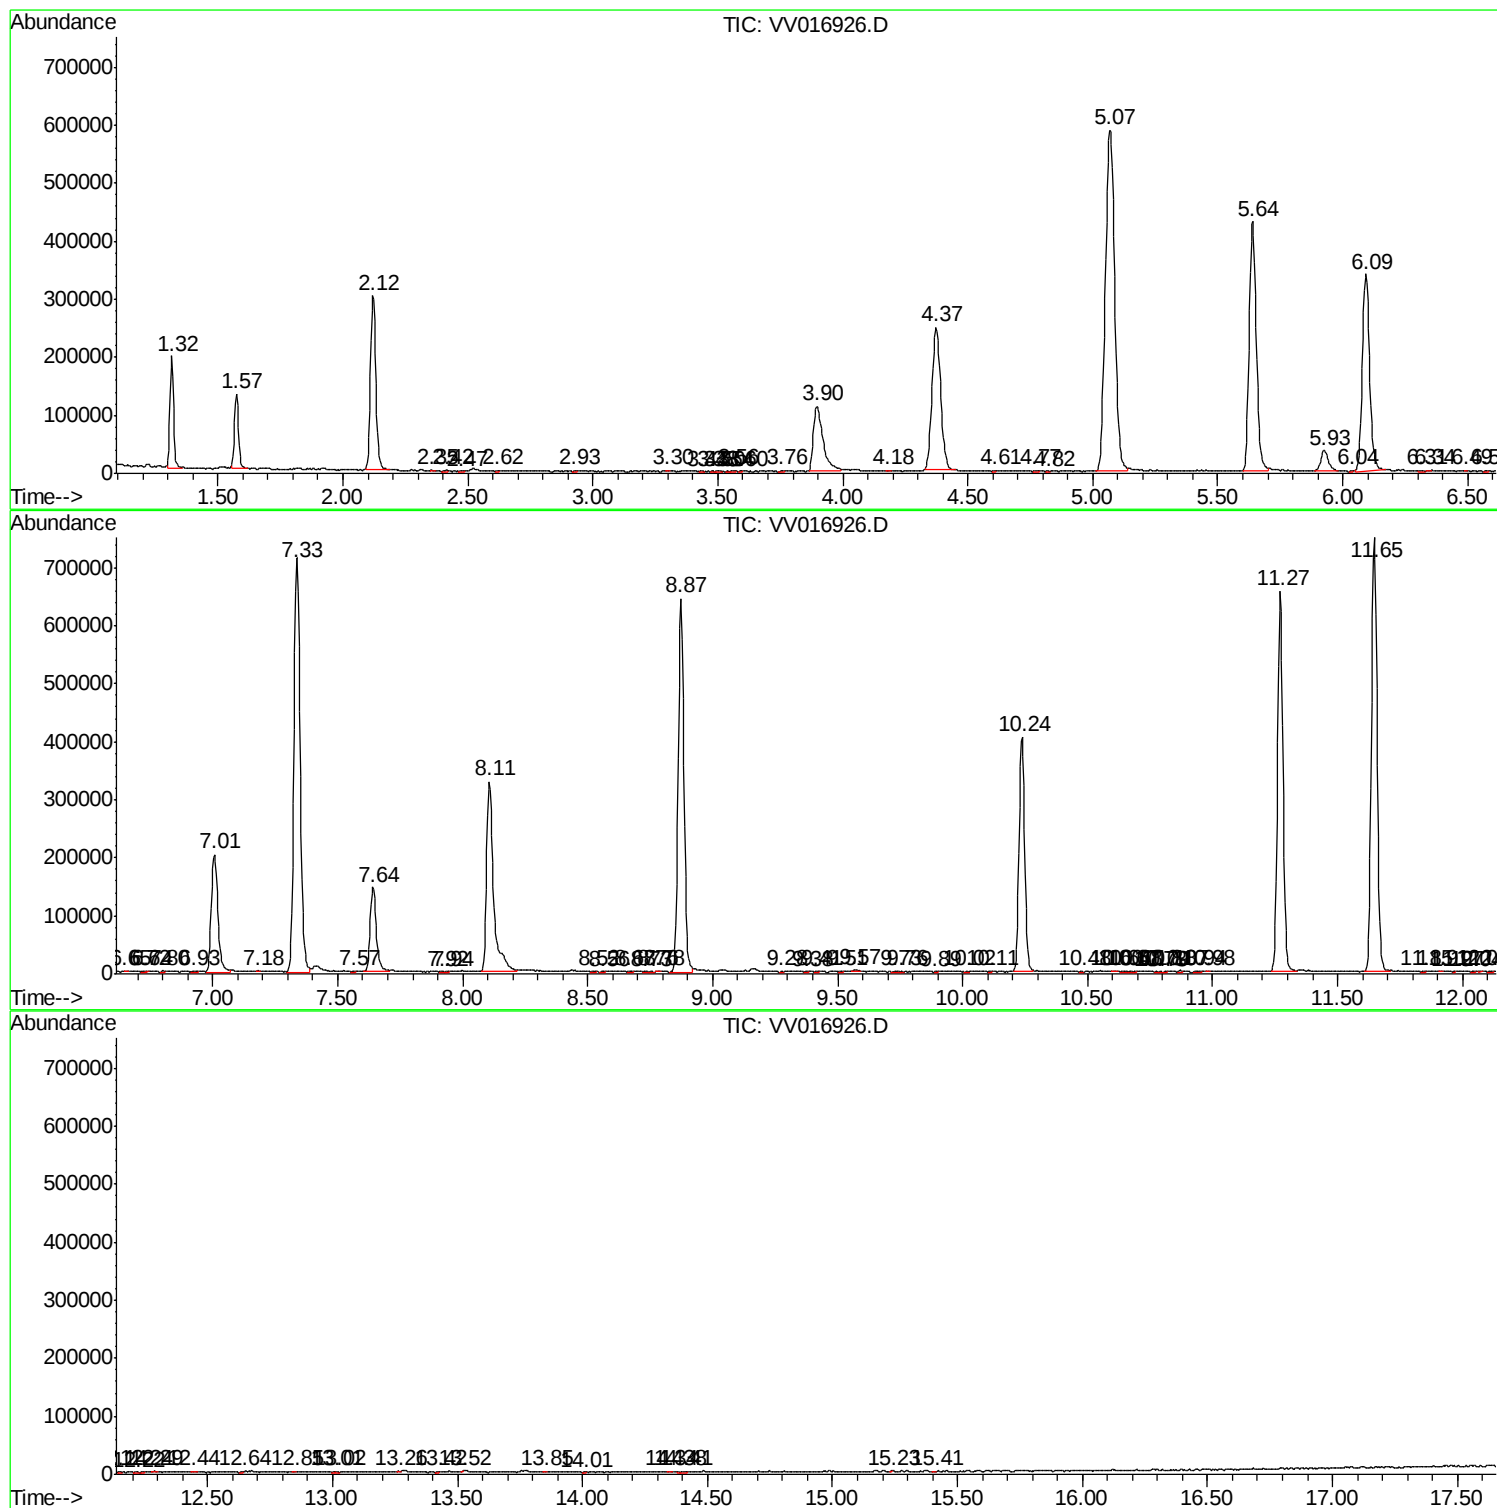

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061520\
Data File : VV016926.D
Acq On : 15 Jun 2020 10:49
Operator : SY/MD
Sample : VV0615WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK87

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV061520\
Data File : VV016926.D
Acq On : 15 Jun 2020 10:49
Operator : SY/MD
Sample : VV0615WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK87

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc