

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016928.D
 Acq On : 15 Jun 2020 11:41
 Operator : SY/MD
 Sample : L2914-14 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	190659	193085	14.94%	1.780%
2	2.116	310	319	342	rVB	283064	423115	32.73%	3.900%
3	2.454	422	424	427	rBV4	1050	695	0.05%	0.006%
4	2.473	427	430	431	rBV3	1435	886	0.07%	0.008%
5	2.856	544	549	552	rBV7	1505	1473	0.11%	0.014%
6	2.904	562	564	569	rBV6	1488	1247	0.10%	0.011%
7	3.026	599	602	605	rBV4	1674	1203	0.09%	0.011%
8	3.161	642	644	646	rBV3	1037	600	0.05%	0.006%
9	3.332	696	697	702	rVB4	1676	1070	0.08%	0.010%
10	3.360	702	706	708	rBV5	1362	975	0.08%	0.009%
11	3.380	708	712	715	rBV4	1902	1285	0.10%	0.012%
12	3.399	715	718	719	rBV3	1538	776	0.06%	0.007%
13	3.454	733	735	737	rBV3	1315	637	0.05%	0.006%
14	3.502	747	750	754	rVB5	1905	1031	0.08%	0.010%
15	3.569	768	771	772	rBV2	1438	656	0.05%	0.006%
16	3.637	789	792	794	rBV4	1454	1127	0.09%	0.010%
17	3.685	805	807	808	rBV2	1769	810	0.06%	0.007%
18	3.743	820	825	826	rBV3	1022	855	0.07%	0.008%
19	3.762	828	831	834	rBV3	1823	1394	0.11%	0.013%
20	3.897	861	873	899	rBV	101007	280749	21.72%	2.588%
21	4.251	980	983	987	rBV6	1566	1331	0.10%	0.012%
22	4.370	1007	1020	1042	rVB	242215	596710	46.16%	5.500%
23	4.650	1103	1107	1108	rBV4	1277	833	0.06%	0.008%
24	4.888	1179	1181	1185	rBV5	1308	840	0.06%	0.008%
25	4.946	1196	1199	1202	rVB4	1328	937	0.07%	0.009%
26	5.071	1219	1238	1243	rBV2	564672	1292784	100.00%	11.915%
27	5.579	1394	1396	1399	rVB3	1582	749	0.06%	0.007%
28	5.640	1402	1415	1435	rBV	451203	896621	69.36%	8.264%
29	5.926	1493	1504	1518	rBV2	27271	57575	4.45%	0.531%
30	6.093	1542	1556	1578	rBV	318967	650718	50.33%	5.997%
31	6.325	1626	1628	1631	rBV3	1168	683	0.05%	0.006%
32	6.511	1684	1686	1689	rBV4	1238	895	0.07%	0.008%
33	6.608	1714	1716	1718	rBV3	1495	633	0.05%	0.006%
34	6.810	1776	1779	1781	rBV4	1259	746	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016928.D
 Acq On : 15 Jun 2020 11:41
 Operator : SY/MD
 Sample : L2914-14 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.907	1805	1809	1810	rBV3	1144	823	0.06%	0.008%
36	6.917	1810	1812	1818	rVB6	2052	1564	0.12%	0.014%
37	6.942	1818	1820	1822	rBV3	2453	1230	0.10%	0.011%
38	7.007	1828	1840	1862	rBV	189596	344810	26.67%	3.178%
39	7.245	1911	1914	1915	rBV3	1292	684	0.05%	0.006%
40	7.267	1915	1921	1922	rBV6	1296	1300	0.10%	0.012%
41	7.335	1928	1942	1959	rBV	668598	1161948	89.88%	10.709%
42	7.640	2027	2037	2052	rBV	134674	225952	17.48%	2.082%
43	7.949	2131	2133	2137	rBV3	1732	726	0.06%	0.007%
44	8.109	2173	2183	2211	rBV2	278253	583742	45.15%	5.380%
45	8.453	2288	2290	2296	rVB7	1801	1213	0.09%	0.011%
46	8.521	2308	2311	2317	rBV6	1563	1648	0.13%	0.015%
47	8.823	2401	2405	2408	rBV6	1791	1640	0.13%	0.015%
48	8.871	2409	2420	2445	rVV	657340	1110425	85.89%	10.234%
49	9.032	2462	2470	2482	rVB	78987	124614	9.64%	1.149%
50	9.283	2539	2548	2557	rBV4	22654	40278	3.12%	0.371%
51	9.826	2705	2717	2726	rBV6	11842	21909	1.69%	0.202%
52	9.884	2726	2735	2745	rBV5	11366	20674	1.60%	0.191%
53	9.994	2765	2769	2770	rBV3	1666	1157	0.09%	0.011%
54	10.109	2794	2805	2811	rBV3	5125	9372	0.72%	0.086%
55	10.174	2819	2825	2826	rBV6	1582	1575	0.12%	0.015%
56	10.238	2834	2845	2860	rVB	387428	601430	46.52%	5.543%
57	10.662	2973	2977	2978	rBV4	1092	787	0.06%	0.007%
58	10.691	2983	2986	2990	rBV5	1620	1421	0.11%	0.013%
59	11.270	3154	3166	3187	rBV	691784	1047110	81.00%	9.651%
60	11.646	3272	3283	3299	rBV	698335	1083828	83.84%	9.989%
61	11.865	3348	3351	3352	rBV3	2091	1015	0.08%	0.009%
62	11.913	3364	3366	3368	rBV3	1246	645	0.05%	0.006%
63	11.974	3383	3385	3386	rBV2	1542	675	0.05%	0.006%
64	12.177	3445	3448	3449	rBV3	1879	912	0.07%	0.008%
65	12.315	3488	3491	3494	rBV5	2232	1457	0.11%	0.013%
66	12.505	3547	3550	3551	rBV2	1407	884	0.07%	0.008%
67	12.514	3551	3553	3554	rBV2	1694	817	0.06%	0.008%
68	12.547	3559	3563	3569	rVB8	2210	2205	0.17%	0.020%
69	12.576	3569	3572	3574	rBV3	1593	1112	0.09%	0.010%
70	12.621	3584	3586	3589	rBV3	1152	662	0.05%	0.006%
71	12.653	3594	3596	3598	rVB3	1562	625	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016928.D
 Acq On : 15 Jun 2020 11:41
 Operator : SY/MD
 Sample : L2914-14 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.868	3661	3663	3665	rBV3	1055	653	0.05%	0.006%
73	12.881	3665	3667	3671	rVB4	2604	1266	0.10%	0.012%
74	12.900	3671	3673	3674	rBV2	1400	724	0.06%	0.007%
75	12.952	3683	3689	3692	rVB6	1822	1377	0.11%	0.013%
76	13.042	3715	3717	3720	rBV4	1546	1003	0.08%	0.009%
77	13.067	3722	3725	3726	rBV3	1346	758	0.06%	0.007%
78	13.206	3766	3768	3773	rBV3	1488	1281	0.10%	0.012%
79	13.293	3787	3795	3797	rBV9	2191	2731	0.21%	0.025%
80	13.434	3836	3839	3842	rBV3	2947	2052	0.16%	0.019%
81	13.524	3860	3867	3870	rBV8	3502	4549	0.35%	0.042%
82	13.810	3952	3956	3958	rBV3	1492	1083	0.08%	0.010%
83	13.820	3958	3959	3963	rVB4	1651	594	0.05%	0.005%
84	13.839	3963	3965	3969	rBV5	767	672	0.05%	0.006%
85	13.948	3997	3999	4003	rBV5	1369	1019	0.08%	0.009%
86	13.984	4008	4010	4013	rBV5	1363	807	0.06%	0.007%
87	14.026	4021	4023	4024	rBV2	1592	675	0.05%	0.006%
88	14.354	4122	4125	4128	rBV3	1324	772	0.06%	0.007%
89	14.373	4128	4131	4132	rBV3	962	614	0.05%	0.006%
90	14.389	4134	4136	4139	rVV4	1410	826	0.06%	0.008%
91	14.418	4143	4145	4147	rVV3	1515	616	0.05%	0.006%
92	14.489	4164	4167	4171	rBV5	1543	1076	0.08%	0.010%
93	14.630	4208	4211	4213	rBV5	1233	759	0.06%	0.007%
94	14.669	4221	4223	4227	rVB4	1594	928	0.07%	0.009%
95	14.688	4227	4229	4230	rBV3	1383	633	0.05%	0.006%
96	14.768	4251	4254	4255	rBV3	1260	651	0.05%	0.006%
97	14.845	4275	4278	4279	rBV4	1522	917	0.07%	0.008%
98	14.952	4309	4311	4315	rVB5	1662	867	0.07%	0.008%
99	15.016	4329	4331	4334	rBV4	1520	956	0.07%	0.009%
100	15.402	4449	4451	4453	rBV3	1374	694	0.05%	0.006%


Sum of corrected areas: 10850146

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061520\
Data File : VV016928.D
Acq On : 15 Jun 2020 11:41
Operator : SY/MD
Sample : L2914-14 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E26

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

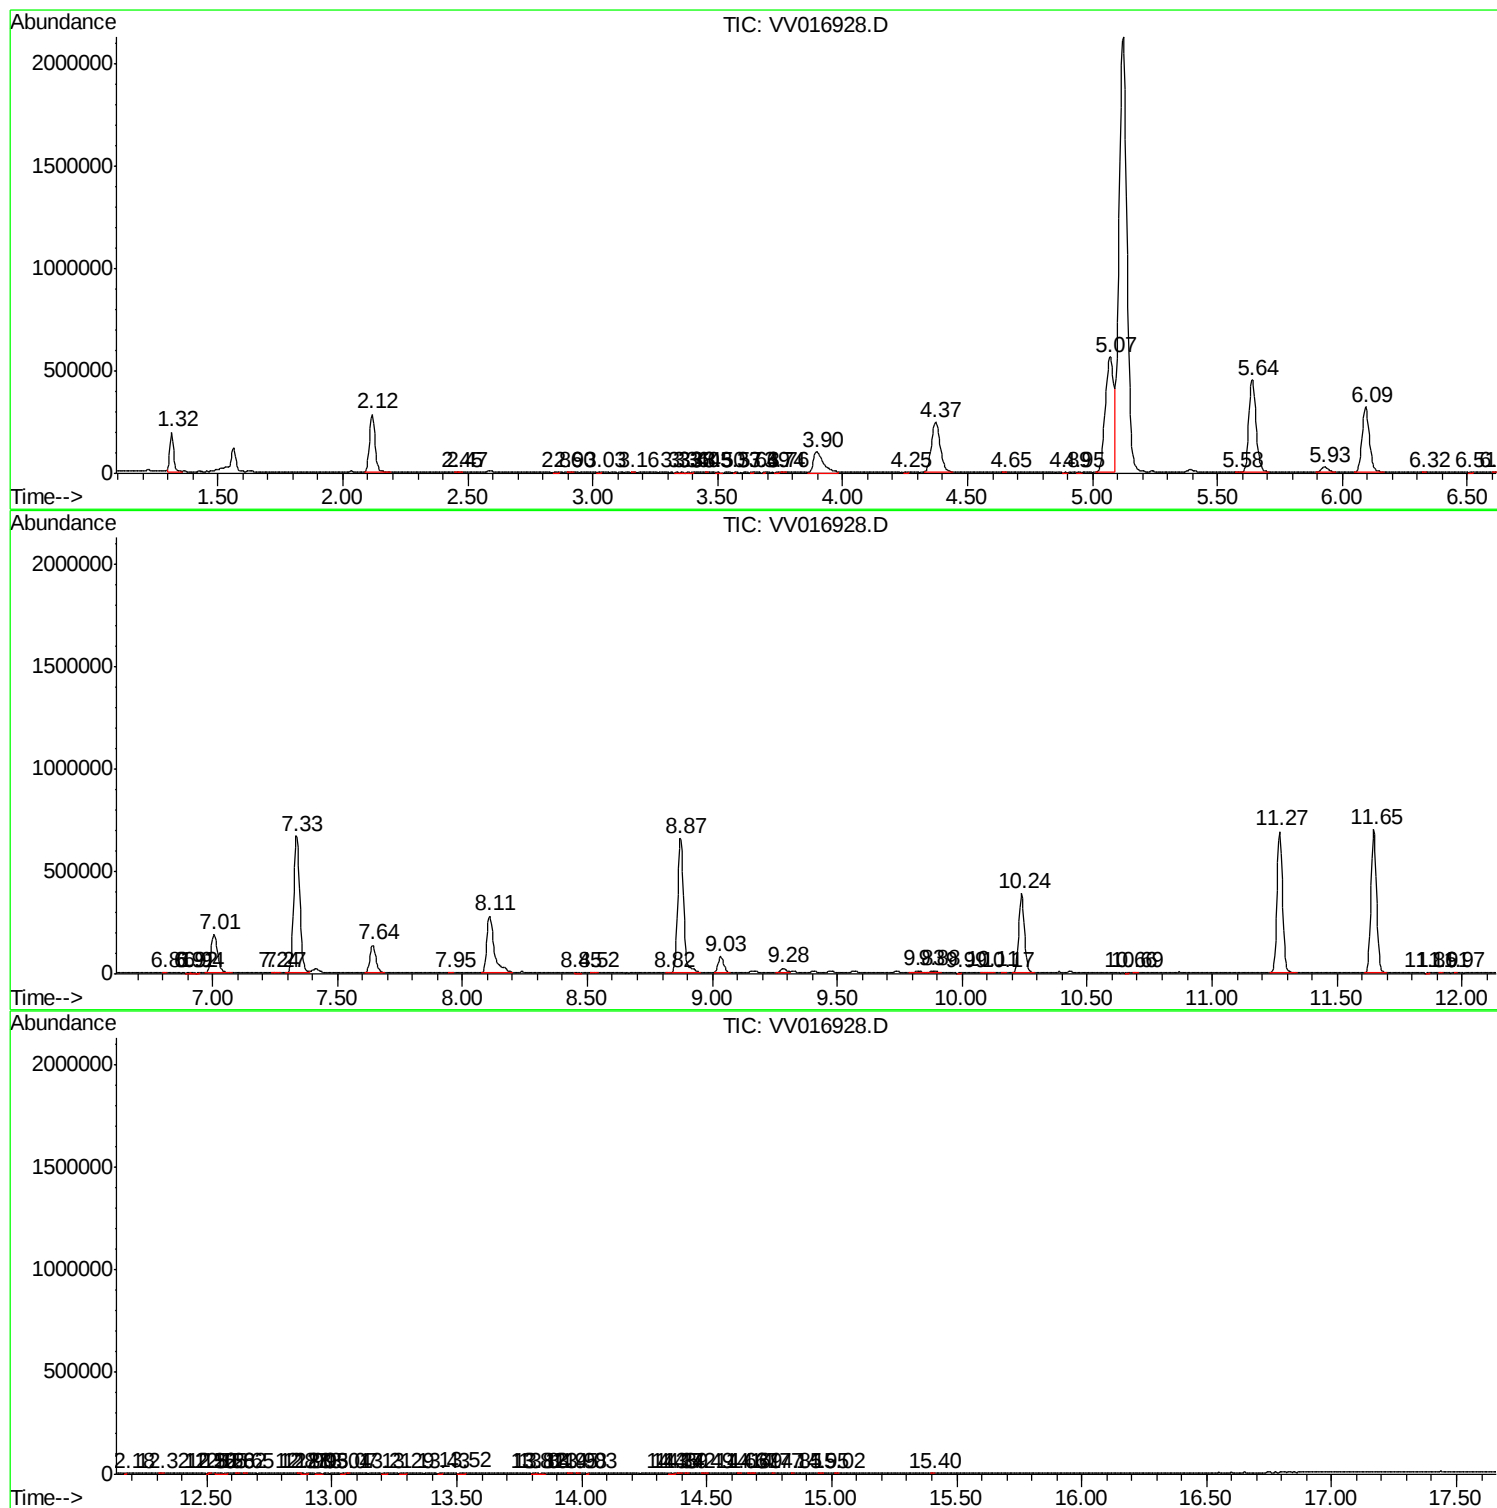

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061520\
Data File : VV016928.D
Acq On : 15 Jun 2020 11:41
Operator : SY/MD
Sample : L2914-14 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E26

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061520\
Data File : VV016928.D
Acq On : 15 Jun 2020 11:41
Operator : SY/MD
Sample : L2914-14 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E26

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
