

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016934.D
 Acq On : 15 Jun 2020 14:15
 Operator : SY/MD
 Sample : L2990-15DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E3YG9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	172610	173030	2.30%	0.945%
2	1.566	143	148	158	rVB	105115	122547	1.63%	0.669%
3	2.119	310	320	336	rVB	273873	413681	5.50%	2.259%
4	2.219	349	351	355	rBV4	1561	1016	0.01%	0.006%
5	2.422	411	414	418	rBV6	1667	1420	0.02%	0.008%
6	2.611	471	473	475	rBV3	1354	826	0.01%	0.005%
7	2.843	543	545	551	rVB4	2227	1233	0.02%	0.007%
8	2.946	573	577	579	rBV2	1624	1090	0.01%	0.006%
9	2.981	586	588	592	rVB4	1242	509	0.01%	0.003%
10	3.013	596	598	600	rBV3	1186	692	0.01%	0.004%
11	3.084	618	620	623	rBV3	1502	880	0.01%	0.005%
12	3.168	643	646	648	rBV3	834	564	0.01%	0.003%
13	3.251	670	672	674	rBV3	1471	778	0.01%	0.004%
14	3.296	683	686	688	rBV4	1541	757	0.01%	0.004%
15	3.367	706	708	711	rVB4	1287	737	0.01%	0.004%
16	3.389	711	715	716	rBV3	2123	1331	0.02%	0.007%
17	3.409	719	721	724	rVB4	1551	822	0.01%	0.004%
18	3.444	730	732	736	rVB4	1738	1287	0.02%	0.007%
19	3.463	736	738	742	rBV3	1187	902	0.01%	0.005%
20	3.508	747	752	755	rVV6	848	774	0.01%	0.004%
21	3.756	826	829	830	rBV3	1181	605	0.01%	0.003%
22	3.901	863	874	899	rBV2	104689	296575	3.95%	1.620%
23	4.142	947	949	951	rBV2	1514	611	0.01%	0.003%
24	4.373	1008	1021	1041	rBV	226032	542454	7.22%	2.962%
25	4.595	1088	1090	1094	rVB5	1739	1160	0.02%	0.006%
26	4.830	1161	1163	1165	rBV3	1318	905	0.01%	0.005%
27	4.856	1169	1171	1172	rBV2	1288	649	0.01%	0.004%
28	4.933	1192	1195	1197	rVB3	1548	890	0.01%	0.005%
29	4.946	1197	1199	1200	rBV2	1229	641	0.01%	0.004%
30	4.984	1209	1211	1213	rVB3	1637	585	0.01%	0.003%
31	5.071	1222	1238	1259	rBV2	552055	1398131	18.60%	7.635%
32	5.640	1401	1415	1440	rBV	450557	900501	11.98%	4.918%
33	5.926	1491	1504	1517	rBV	27018	61568	0.82%	0.336%
34	6.093	1539	1556	1579	rBV	320832	648725	8.63%	3.543%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016934.D
 Acq On : 15 Jun 2020 14:15
 Operator : SY/MD
 Sample : L2990-15DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E3YG9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.540	1693	1695	1699	rVB4	1294	966	0.01%	0.005%
36	6.585	1706	1709	1710	rBV3	1540	724	0.01%	0.004%
37	6.605	1713	1715	1719	rVB3	1948	1183	0.02%	0.006%
38	6.627	1719	1722	1724	rBV4	1806	1302	0.02%	0.007%
39	6.720	1748	1751	1753	rVB4	1375	593	0.01%	0.003%
40	6.769	1763	1766	1768	rBV4	1512	1085	0.01%	0.006%
41	6.804	1775	1777	1779	rBV3	1304	677	0.01%	0.004%
42	6.862	1792	1795	1797	rBV3	2263	1313	0.02%	0.007%
43	6.900	1804	1807	1809	rBV4	1099	553	0.01%	0.003%
44	7.007	1828	1840	1861	rBV	186783	337520	4.49%	1.843%
45	7.235	1908	1911	1914	rBV4	1788	1249	0.02%	0.007%
46	7.338	1932	1943	1954	rBV	666102	1132182	15.06%	6.183%
47	7.409	1954	1965	1991	rVB	4450984	7515954	100.00%	41.045%
48	7.640	2029	2037	2054	rVB	131819	214952	2.86%	1.174%
49	8.109	2172	2183	2216	rBV	301261	607099	8.08%	3.315%
50	8.560	2320	2323	2324	rBV2	1400	691	0.01%	0.004%
51	8.569	2324	2326	2330	rVB5	1922	946	0.01%	0.005%
52	8.585	2330	2331	2334	rBV3	2023	958	0.01%	0.005%
53	8.688	2360	2363	2368	rVB7	1988	1441	0.02%	0.008%
54	8.730	2371	2376	2378	rBV5	1326	1052	0.01%	0.006%
55	8.746	2378	2381	2382	rBV3	1433	731	0.01%	0.004%
56	8.788	2391	2394	2396	rBV3	986	583	0.01%	0.003%
57	8.871	2409	2420	2435	rBV	676197	1081128	14.38%	5.904%
58	9.035	2465	2471	2484	rVB	27839	44412	0.59%	0.243%
59	9.161	2500	2510	2522	rBV	38557	65440	0.87%	0.357%
60	9.341	2564	2566	2570	rVB4	1407	840	0.01%	0.005%
61	9.370	2570	2575	2579	rVB8	1554	1215	0.02%	0.007%
62	9.399	2582	2584	2587	rBV3	1365	664	0.01%	0.004%
63	9.463	2602	2604	2605	rBV2	1483	555	0.01%	0.003%
64	9.569	2630	2637	2644	rVV9	6045	9571	0.13%	0.052%
65	9.775	2698	2701	2706	rBV8	1395	1559	0.02%	0.009%
66	9.859	2724	2727	2730	rVB4	1346	636	0.01%	0.003%
67	9.952	2753	2756	2759	rBV4	2242	1938	0.03%	0.011%
68	10.023	2773	2778	2780	rVB4	1440	1167	0.02%	0.006%
69	10.035	2780	2782	2784	rBV3	2022	1271	0.02%	0.007%
70	10.238	2834	2845	2860	rBV	377810	588813	7.83%	3.216%
71	10.363	2881	2884	2886	rBV4	1576	925	0.01%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016934.D
 Acq On : 15 Jun 2020 14:15
 Operator : SY/MD
 Sample : L2990-15DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E3YG9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.437	2904	2907	2910	rBV4	1512	982	0.01%	0.005%
73	10.466	2914	2916	2919	rBV4	1633	630	0.01%	0.003%
74	10.556	2942	2944	2946	rBV2	1367	730	0.01%	0.004%
75	10.717	2992	2994	2996	rBV3	2004	872	0.01%	0.005%
76	10.926	3056	3059	3061	rBV5	1708	1194	0.02%	0.007%
77	11.103	3110	3114	3115	rBV4	1051	657	0.01%	0.004%
78	11.270	3155	3166	3182	rBV	671180	1024302	13.63%	5.594%
79	11.350	3188	3191	3194	rBV5	2745	1787	0.02%	0.010%
80	11.585	3262	3264	3266	rBV3	1008	519	0.01%	0.003%
81	11.646	3272	3283	3308	rVB	677272	1052639	14.01%	5.749%
82	11.952	3376	3378	3380	rVB3	1448	601	0.01%	0.003%
83	12.196	3450	3454	3458	rBV5	1381	1354	0.02%	0.007%
84	12.251	3469	3471	3473	rBV3	2504	1319	0.02%	0.007%
85	12.431	3525	3527	3530	rVB4	2005	831	0.01%	0.005%
86	12.457	3533	3535	3538	rBV3	1376	760	0.01%	0.004%
87	12.624	3584	3587	3590	rBV5	1885	1446	0.02%	0.008%
88	12.939	3683	3685	3689	rVB4	1804	953	0.01%	0.005%
89	12.971	3689	3695	3698	rBV9	1868	1971	0.03%	0.011%
90	13.177	3757	3759	3761	rBV3	1636	931	0.01%	0.005%
91	13.244	3777	3780	3787	rBV6	2255	2291	0.03%	0.013%
92	13.366	3815	3818	3821	rBV4	871	614	0.01%	0.003%
93	13.479	3848	3853	3856	rBV7	1655	1459	0.02%	0.008%
94	13.566	3878	3880	3884	rBV5	1437	874	0.01%	0.005%
95	13.646	3901	3905	3909	rBV5	2318	1982	0.03%	0.011%
96	13.765	3937	3942	3946	rBV7	1679	1638	0.02%	0.009%
97	13.849	3964	3968	3970	rBV5	1687	862	0.01%	0.005%
98	13.881	3976	3978	3980	rBV3	1326	703	0.01%	0.004%
99	14.186	4070	4073	4074	rBV3	1416	748	0.01%	0.004%
100	14.794	4257	4262	4267	rBV9	2199	3101	0.04%	0.017%


Sum of corrected areas: 18311514

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061520\
Data File : VV016934.D
Acq On : 15 Jun 2020 14:15
Operator : SY/MD
Sample : L2990-15DL 200X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E3YG9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

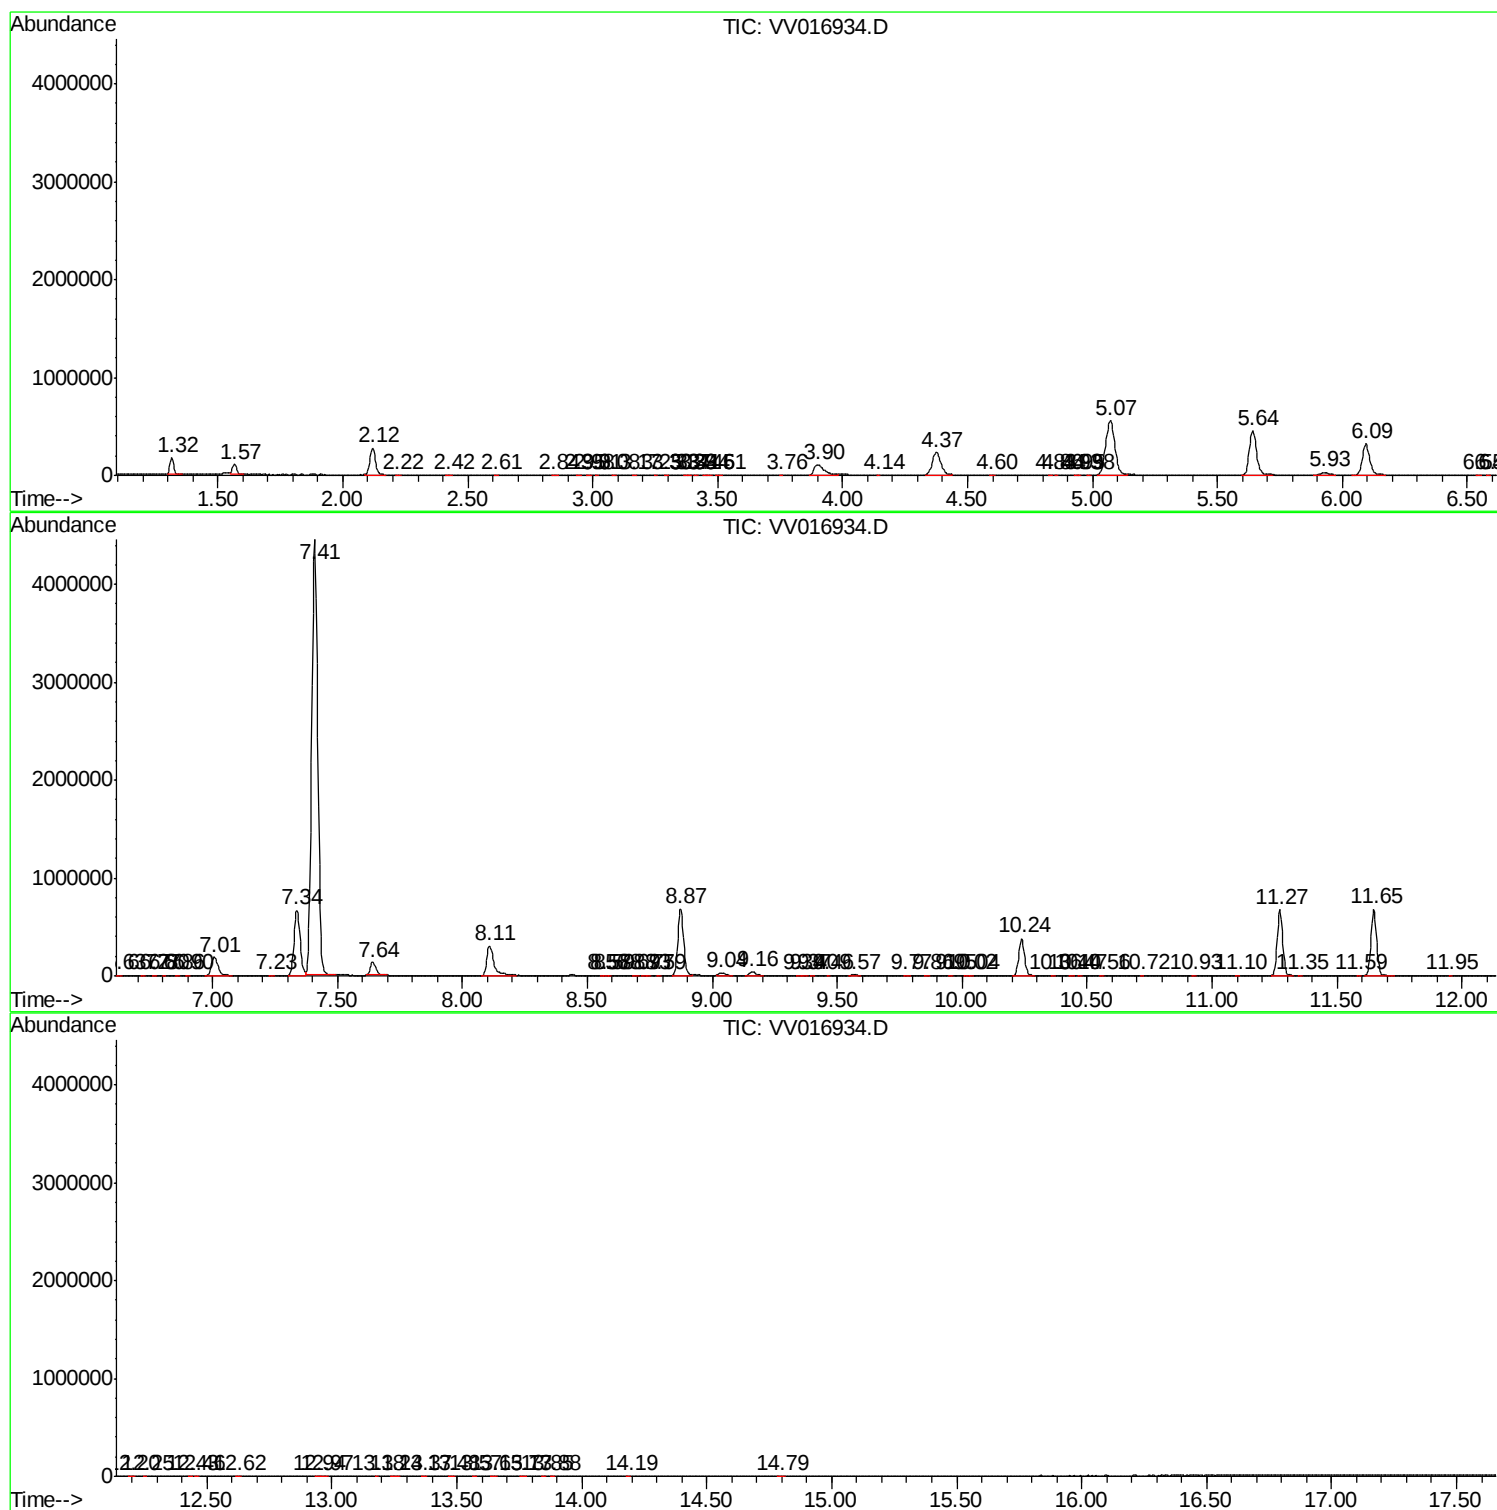

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061520\
Data File : VV016934.D
Acq On : 15 Jun 2020 14:15
Operator : SY/MD
Sample : L2990-15DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E3YG9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV061520\
Data File : VV016934.D
Acq On : 15 Jun 2020 14:15
Operator : SY/MD
Sample : L2990-15DL 200X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
E3YG9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc